

User's Manual

CentriVap® Centrifugal Concentrators and Cold Traps

Models

78100-00	78110-00	79820-00
78100-01	78110-01	79820-01
78100-02	74600-00	79830-00
78100-03	74600-01	79830-01
		79840-00
		79840-01
		74750-00
		74750-01

Register your product online at
www.labconco.com/productreg.html
or return the attached card and
receive **FREE LabbyWear™!**



Labconco's Mascot,
Labby the LABster



*Protecting your
laboratory environment*

LABCONCO®

LABCONCO CORPORATION
8811 PROSPECT AVENUE
KANSAS CITY, MO 64132-2696
800-821-5525, 816-333-8811
FAX 816-363-0130
E-MAIL labconco@labconco.com
HOME PAGE www.labconco.com

Copyright Information

Copyright © 2000 Labconco Corporation. All rights reserved.

Labconco Corporation
8811 Prospect Avenue
Kansas City, Missouri 64132

The information contained in this manual and the accompanying product are copyrighted and all rights are reserved by Labconco Corporation. Labconco Corporation reserves the right to make periodic design changes without obligation to notify any person or entity of such change.

CentriVap® is a registered trademark of Labconco Corporation.

Warranty

Labconco provides a warranty on all parts and factory workmanship. The warranty includes areas of defective material and workmanship, provided such defect results from normal and proper use of the equipment.

The warranty for all Labconco products will expire one year from date of installation or two years from date of shipment from Labconco, whichever is sooner, except the following:

- Purifier® Delta™ Series Biological Safety Cabinets, which carry a three-year warranty from date of installation or four years from date of shipment from Labconco, whichever is sooner.
- Carts carry a lifetime warranty.
- Glassware is not warranted from breakage when dropped or mishandled.

This limited warranty covers parts and labor, but not transportation and insurance charges. In the event of a warranty claim, contact Labconco Corporation or the dealer who sold you the product. If the cause is determined to be a manufacturing fault, the dealer or Labconco Corporation will repair or replace all defective parts to restore the unit to operation. Under no circumstances shall Labconco Corporation be liable for indirect, consequential, or special damages of any kind. This statement may be altered by a specific published amendment. No individual has authorization to alter the provisions of this warranty policy or its amendments. Lamps and filters are not covered by this warranty. Damage due to corrosion or accidental breakage is also not covered.

Limitation of Liability

The disposal and/or emission of substances used in connection with this equipment may be governed by various federal, state, or local regulations. All users of this equipment are required to become familiar with any regulations that apply in the user's area concerning the dumping of waste materials in or upon water, land, or air and to comply with such regulations. Labconco Corporation is held harmless with respect to user's compliance with such regulations.

Contacting Labconco Corporation



If you have questions that are not addressed in this manual, or if you need technical assistance, contact Labconco's Customer Service Department or Labconco's Product Service Department at 1-800-821-5525 or 1-816-333-8811, between the hours of 7:00 a.m. and 6:00 p.m., Central Standard Time.

Visit Labconco's web site at: <http://www.labconco.com> or email Labconco at: labconco@labconco.com.

TABLE OF CONTENTS

CHAPTER 1: INTRODUCTION	1
About This Manual	2
Typographical Conventions	3
Your Next Step	4
CHAPTER 2: PREREQUISITES	5
Electrical Requirements	6
Location and Exhaust Requirements	6
Vacuum Pump Requirements	7
Vacuum Line Traps	8
Space Requirements	8
Your Next Step	8
CHAPTER 3: GETTING STARTED	9
Unpacking Your CentriVap	10
CentriVap Components	10
Setting Up Your CentriVap	13
Emergency Access Into the Chamber	13
Component Orientation & Hose Connections	13
Exhaust Port	15
Electrical Connection	15
Rotor Installation	15
Ground Wire	15
Solvent Safety Precautions	16
Your Next Step	18
CHAPTER 4: USING YOUR CENTRIVAP	19
Planning	20
Glassware Selection	20
Loading Glassware Into the CentriVap	20
Heat Setting Guidelines	20
Time Setting Guidelines	21
Heat Boost Operation	21

CentriVap Controls	22
Operating the CentriVap Controls	23
Operating The CentriVap	24
Operational Notes	25
Interrupting a Cycle After it Has Begun	26
CHAPTER 5: MAINTAINING YOUR CENTRIVAP	27
CHAPTER 6: MODIFYING YOUR CENTRIVAP	29
Installing a Glass Lid	29
Installing a Secondary Chemical Trap	30
Installing a CentriZap Strobe Light	32
Installing a Glass Trap in the Cold Trap	33
CHAPTER 7: TROUBLESHOOTING	35
APPENDIX A: CENTRIVAP COMPONENTS	39
APPENDIX B: CENTRIVAP DIMENSIONS	47
APPENDIX C: CENTRIVAP SPECIFICATIONS	51
Wiring Diagram Concentrator (115V)	53
Wiring Diagram Concentrator (230V)	54
Wiring Diagram Cold Trap (–55°) (115V & 230V)	55
Evaporation Rates	56
APPENDIX D: CENTRIVAP ACCESSORIES	59
DECLARATION OF CONFORMITY	63

CHAPTER 1

INTRODUCTION

Congratulations on your purchase of a Labconco CentriVap Concentrator System. Models are available for operation on 115V or 230V.

The CentriVap Concentrator, when combined with the CentriVap Cold Trap, uses centrifugal force with heat and vacuum to rapidly evaporate and condense solvents from biological and analytical samples. Centrifugation eliminates bumping and foaming as vacuum is applied and also concentrates the solute in the bottom of the vial. This allows recovery of solutes from sample volumes as small as a few microliters. The Concentrator is equipped with a 300 watt heater to speed evaporation by warming the chamber during processing. A timed outlet for the vacuum pump connection delays the start of the pump until the rotor reaches operating speed. A safety switch prevents the concentrator from starting when the lid is in the open position and a latch prevents the lid from being opened while the rotor is turning. The compact, low profile design allows the Concentrator to be placed on a bench top or other laboratory work surface.

The microprocessor which controls the operation of the heater and the motor provides excellent regulation and reproducibility of protocols. The end of the run can be signaled by a manually preset timer. Nine different protocols can be stored in memory so exact test parameters can be easily repeated.

As the companion to the Concentrator, the CentriVap Cold Trap protects the vacuum pump by trapping moisture, vapors and corrosive fumes as they evaporate from the samples. The CFC free refrigeration system reduce the temperature of the Cold Trap to -55°C . The stainless steel trap is used for aqueous and organic applications. For corrosive applications, the optional Glass Trap insert should be used. The 230V models comply with CE regulations.

About This Manual

This manual is designed to help you learn how to install, use, and maintain your CentriVap. Instructions for performing routine maintenance and making minor modifications to your CentriVap are also included.

Chapter 1: Introduction provides a brief overview of the CentriVap, explains the organization of the manual, and defines the typographical conventions used in the manual.

Chapter 2: Prerequisites explains what you need to do to prepare your site before you install your CentriVap. Electrical and exhaust requirements are discussed.

Chapter 3: Getting Started contains the information you need to properly unpack, inspect and install your CentriVap.

Chapter 4: Using Your CentriVap discusses the basic operation of your CentriVap. Information on how to arrange the samples inside your CentriVap and select an operating cycle is included.

Chapter 5: Maintaining Your CentriVap explains how to perform routine maintenance on your CentriVap.

Chapter 6: Modifying Your CentriVap describes how to install the optional glass lid.

Chapter 7: Troubleshooting contains a table of problems you may encounter while using your CentriVap, including the probable causes of the problems, and suggested corrective actions.

Appendix A: CentriVap Components contains labeled diagrams of the components of the CentriVap.

Appendix B: CentriVap Dimensions contains comprehensive diagrams showing the dimensions for the CentriVap.

Appendix C: CentriVap Specifications contains product specifications. Wiring diagrams for both the 115V and 230V CentriVap are also included.

Appendix D: CentriVap Accessories lists the part numbers and descriptions of all of the accessories available for your CentriVap.

Typographical Conventions

Recognizing the following typographical conventions will help you understand and use this manual:

- Book, chapter, and section titles are shown in italic type (e.g., *Chapter 3: Getting Started*).
- Steps required to perform a task are presented in a numbered format.
- Comments located in the margins provide suggestions, reminders, and references.
- Critical information is presented in boldface type in paragraphs that are preceded by the exclamation icon. Failure to comply with the information following an exclamation icon may result in injury to the user or permanent damage to your CentriVap.
- Important information is presented in capitalized type in paragraphs that are preceded by the pointer icon. It is imperative that the information contained in these paragraphs be thoroughly read and understood by the user.



Your Next Step

If your CentriVap needs to be installed, proceed to *Chapter 2: Prerequisites* to ensure your installation site meets all of the requirements. Then, go to *Chapter 3: Getting Started* for instructions on how to install your CentriVap and make all of the necessary connections.

For information on the operational characteristics of your CentriVap, go to *Chapter 4: Using Your CentriVap*.

If your CentriVap is installed and you need to perform routine maintenance on the CentriVap, proceed to *Chapter 5: Maintaining Your CentriVap*.

For information on making modifications to the configuration of your CentriVap go to *Chapter 6: Modifying Your CentriVap*.

Refer to *Chapter 7: Troubleshooting* if you are experiencing problems with your CentriVap.

CHAPTER 2

PREREQUISITES

Before you install your CentriVap, you need to prepare your site for installation. Carefully examine the location where you intend to install your CentriVap. You must be certain that the area is level and of solid construction. In addition, an exhaust means must be provided. An electrical source must be located near the installation site.

Carefully read this chapter to learn:

- the electrical supply requirements.
- the exhaust requirements.
- the vacuum pump requirements.

Refer to *Appendix C: CentriVap Specifications* for complete CentriVap electrical and environmental conditions, specifications and requirements.



The CentriVap has not been evaluated by an approval agency for the use of biological, radiotoxins or flammable liquids or materials.

Electrical Requirements

The CentriVap Concentrator requires a dedicated grounded electrical outlet. This outlet requires a 15 Amp circuit breaker or fuse for models rated at 115V (60 Hz). An 8 Amp circuit breaker or fuse is required for models rated at 230V (50/60 Hz). 115V models are equipped with a 15 Amp NEMA 5-15P plug. 230V models are not equipped with a plug. It will be necessary to install a plug to match the available receptacle.

The CentriVap Cold Trap requires a dedicated electrical outlet. Models 74600-00 and 78110-00 require a 15 Amp circuit breaker or fuse rated at 115V (60 Hz). Models 74600-01 and 78110-01 require an 8 Amp circuit breaker or fuse rated at 230V (50/60 Hz). 115V models are equipped with a 15 Amp NEMA 5-15P plug. 230V models are not equipped with a plug. It will be necessary to install a plug to match the available receptacle.

It is recommended that an emergency switch for disconnecting the mains in the case of a malfunction be located remote from the CentriVap, preferably outside the room in which the CentriVap is housed, or adjacent to the exit from that room.

Location and Exhaust Requirements

The CentriVap System should be located within a fume hood if hazardous or flammable solvents are used. In all cases, regardless of the solvent used, it is strongly recommended that the vacuum pump is vented in a fume hood. An accessory secondary trap is available to minimize the exhausting of solvents into the atmosphere. This does not, however, negate the need to exhaust the vacuum pump into a fume hood.

Vacuum Pump Requirements

A vacuum pump must be provided by the user. A vacuum pump with a free air flow rate of 113 liters per minute and 0.2×10^{-3} mbar blank off pressure is adequate for aqueous samples. More volatile samples can be satisfactorily processed using a diaphragm pump with a free airflow of 42 liters per minute and 200 mbar vacuum. The inlet fitting on the vacuum pump must be suitable for 0.50 I.D. hose.

Vacuum pumps used with 115V models should be equipped with a 115V, 15 Amp NEMA 5-15P plug. Vacuum pumps used with 230V models should be equipped with a “reverse” IEC 320 plug. This will allow the vacuum pump to be plugged into the receptacle on the back of the CentriVap.



TO INSURE THAT AGGRESSIVE SAMPLES USED IN THE CENTRIVAP DO NOT DAMAGE THE VACUUM PUMP, IT IS RECOMMENDED THAT ALL INTERNAL WETTED PARTS ARE TEFLON®* OR TEFLON COATED.



CAUTION: When selecting the vacuum pump it is very important to consider the flammability of the solvent that will be used. If the solvents are flammable, an explosion proof vacuum pump or one suitable for the solvents to be processed is recommended.

*Teflon® is a registered trademark of DuPont

Vacuum Line Traps

When using a mechanical pump which is not corrosion resistant, the CentriVap Cold Trap or equivalent trap must be used in the vacuum line to prevent damage from solvent vapors. When evaporating acids, it is advisable to include a soda lime acid secondary trap in the vacuum line. This adds additional protection for the pump.



Several components within the CentriVap are made from stainless steel or aluminum and can be degraded if exposed to acids. Before evaporating acids, be sure to contact Labconco.

A moisture trap, solvent trap and radioisotope trap are also available. Refer to *Appendix D: CentriVap Accessories* for ordering information.

Space Requirements

Refer to *Appendix C: CentriVap Specifications* for dimensional drawings of the CentriVap.

Your Next Step

After you have determined that the location for your CentriVap accommodates the installation and operational requirements, you are ready to unpack and install your CentriVap. Proceed to *Chapter 3: Getting Started*.

CHAPTER 3

GETTING STARTED

Now that the site for your CentriVap is properly prepared, you are ready to unpack, inspect, install, and test your CentriVap. Read this chapter to learn how to:

- unpack and move your CentriVap.
- set up your CentriVap.
- connect the electrical supply source to your CentriVap.
- properly exhaust your CentriVap.
- safely use solvents with your CentriVap.




The CentriVap Concentrator weighs over 42 lbs. (19 Kg). The carton allows for lifting with a mechanical lift truck or hand truck. If you must lift the CentriVap manually, use at least two (2) persons and follow safe lifting guidelines.

The CentriVap Cold Trap weighs over 70 lbs. (33 Kg). The carton allows for lifting with a mechanical lift truck or hand truck. If you must lift the Cold Trap manually, use at least two (2) persons and follow safe lifting guidelines.

Unpacking Your CentriVap

The United States Interstate Commerce Commission rules require that claims be filed with the delivery carrier within fifteen (15) days of delivery.

Carefully unpack your CentriVap and inspect it for damage that may have occurred in transit. If your CentriVap is damaged, notify the delivery carrier immediately and retain the entire shipment intact for inspection by the carrier.



DO NOT RETURN GOODS WITHOUT THE PRIOR AUTHORIZATION OF LABCONCO. UNAUTHORIZED RETURNS WILL NOT BE ACCEPTED.



IF YOUR CENTRIVAP WAS DAMAGED IN TRANSIT, YOU MUST FILE A CLAIM DIRECTLY WITH THE FREIGHT CARRIER. LABCONCO CORPORATION AND ITS DEALERS ARE NOT RESPONSIBLE FOR SHIPPING DAMAGE.

Do not discard the carton or packing material for your CentriVap until you have checked all of the components and installed and tested the CentriVap.

CentriVap Components

As previously mentioned, the CentriVap System is available in 115V or 230V. Locate the model of CentriVap you received in the following table. Verify that the components listed are present and undamaged.

Concentrator

Catalog #	Product Description
78100-00	CentriVap Concentrator – 115V
78100-10	CentriVap Concentrator – 230V
78100-02	CentriVap Concentrator with Heat Boost – 115V
78100-03	CentriVap Concentrator with Heat Boost – 230V

Plus the Following:

Part #	Component Description
74614-00	User's Manual
13345-00	Power Cord – 115V
	or
13341-00	Power Cord – 230V
78286-06	Tubing
14888-00	Clamp (2)

Cold Trap

Catalog #	Product Description
78110-00	CentriVap Cold Trap – 115V
78110-01	CentriVap Cold Trap – 230V

Plus the Following:

Part #	Component Description
74614-00	User's Manual
13345-00	Power Cord – 115V
	or
13341-00	Power Cord – 230V
74646-00	Wire Assembly
78286-06	Tubing
14888-00	Clamp (2)
79814-00	Insulation – Cover
78735-00	Cover Assembly

Catalog #	Product Description
74600-00	CentriVap Cold Trap – 115V
74600-01	CentriVap Cold Trap – 230V

Plus the Following:

Part #	Component Description
74614-00	User's Manual
13345-00	Power Cord – 115V
	or
13341-00	Power Cord – 230V
74646-00	Wire Assembly
78286-06	Tubing
14888-00	Clamp (2)
79814-00	Insulation – Cover
78735-00	Cover Assembly

Systems

Catalog #	Product Description
-----------	---------------------

79820-00	Aqueous System – 115V
----------	-----------------------

79820-01	Aqueous System – 230V
----------	-----------------------

Plus the Following:

Part #	Component Description
--------	-----------------------

78100-00	CentriVap Concentrator – 115V
----------	-------------------------------

or

78100-01	CentriVap Concentrator – 230V
----------	-------------------------------

78110-00	CentriVap Cold Trap – 115V
----------	----------------------------

or

78110-01	CentriVap Cold Trap – 230V
----------	----------------------------

74609-00	Cannister Assembly
----------	--------------------

78149-00	Cartridge – Moisture Trap
----------	---------------------------

74550-00	Rotor – 15ml
----------	--------------

Catalog #	Product Description
-----------	---------------------

79830-00	Acid System – 115V
----------	--------------------

79830-01	Acid System – 230V
----------	--------------------

Plus the Following:

Part #	Component Description
--------	-----------------------

78100-00	CentriVap Concentrator – 115V
----------	-------------------------------

or

78100-01	CentriVap Concentrator – 230V
----------	-------------------------------

78110-00	CentriVap Cold Trap – 115V
----------	----------------------------

or

78110-01	CentriVap Cold Trap – 230V
----------	----------------------------

74609-00	Cannister Assembly
----------	--------------------

78148-00	Cartridge – Acid Trap
----------	-----------------------

74550-00	Rotor – 15ml
----------	--------------

78734-00	Glass Trap Assembly
----------	---------------------

Catalog #	Product Description
-----------	---------------------

79840-00	Solvent System – 115V
----------	-----------------------

79840-01	Solvent System – 230V
----------	-----------------------

Plus the Following:

Part #	Component Description
--------	-----------------------

78100-00	CentriVap Concentrator – 115V
----------	-------------------------------

or

78100-01	CentriVap Concentrator – 230V
----------	-------------------------------

78110-00	CentriVap Cold Trap – 115V
----------	----------------------------

or

78110-01	CentriVap Cold Trap – 230V
----------	----------------------------

74609-00	Cannister Assembly
----------	--------------------

78152-00	Cartridge – Solvent Trap
----------	--------------------------

74550-00	Rotor – 15ml
----------	--------------

If you do not receive one or more of the components listed for your CentriVap, or if any of the components are damaged, contact Labconco Corporation immediately for further instructions.

Setting Up Your CentriVap

After you verify receipt of the proper components, move your CentriVap to the level and sturdy location where you want to install it. There is no need to secure the CentriVap to the work surface. Then, follow the steps listed below.

Emergency Access Into the Chamber

The CentriVap is designed to prevent access to the chamber in the event of a power disruption. If it is necessary to open the lid when there is no electrical power connected to the CentriVap, insert a small screwdriver or similar instrument into the small round hole on the left side of the case near the top behind the control panel. This will unlock the lid latch mechanism. While holding the screwdriver in place, raise the lid with the other hand.




Never attempt to defeat the latch or open the lid while the CentriVap is running.

Component Orientation & Hose Connections

The relative position of the CentriVap Concentrator, Cold Trap and the vacuum pump may be as shown or may be reversed. The refrigeration system in the Cold Trap exhausts air through the rear of the cabinet. A minimum of 3" should be allowed between the back of the Cold Trap and the adjacent wall surface and between the sides of the Cold Trap and the adjacent

wall surfaces. Restriction of the airflow through the cabinet during operation could adversely affect performance.

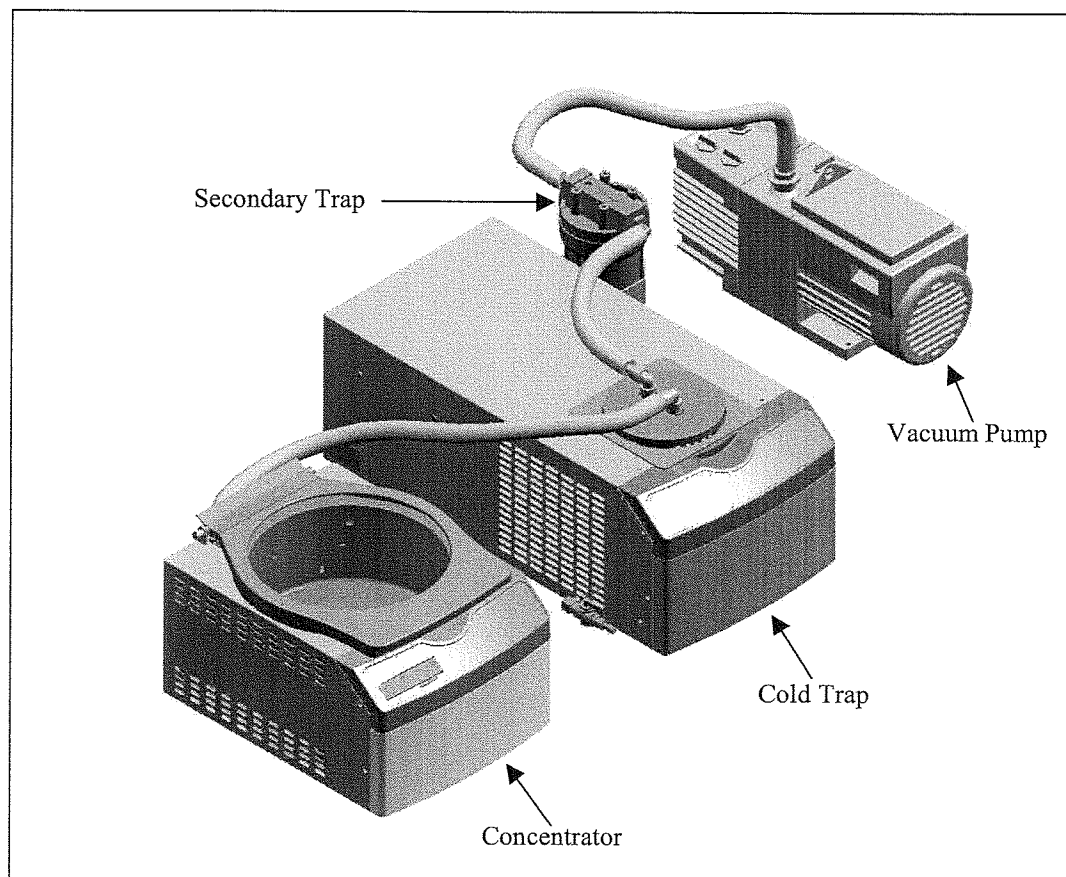

After positioning the components, it is necessary to join the system together using the hoses provided. Attach one hose to the .50 diameter tube that extends out the back of the Concentrator. Attach the other end of this hose to one of the barb fittings on the Cold Trap Cover Assembly. Clamp securely with the clamps supplied. Attach another hose to the remaining barb fitting on the Cold Trap Cover Assembly and clamp securely. If the accessory Secondary Trap is not used, attach the other end of the hose to the inlet port on the vacuum pump. If the accessory Secondary Trap is used, install the Secondary Trap as explained in *Chapter 6: Modifying Your CentriVac*. Then attach the hose from the Cold Trap Cover Assembly to the “out” connector on the

Secondary Trap. Clamp securely. Attach another hose from the remaining connector on the Secondary Trap to the inlet port on the vacuum pump and clamp securely.

Exhaust Port

If the CentriVap is not located in a fume hood, attach one end of a user supplied hose to the exhaust port on the vacuum pump. Clamp securely. Route the other end to a fume hood or other laboratory ventilation device.

Electrical Connection

Plug the power cord into the receptacle on the back of the CentriVap Concentrator and plug the other end into a suitable power receptacle. Plug the power cord into the receptacle on the back of the CentriVap Cold Trap and plug the other end into a suitable power receptacle. Plug the power cord from the vacuum pump into the receptacle on the back of the Concentrator. If the vacuum pump has an off/on switch, turn the switch on. The vacuum pump will be controlled by the Concentrator.

Rotor Installation

Place the rotor onto the shaft of the Concentrator. Rotate the rotor slightly to engage the drive pin in the shaft with the slots in the rotor hub. The top of the shaft should be in line with the top of the rotor hub.



Do not use a rotor if it shows any signs of damage.

Ground Wire

Attach one end of the included ground wire to the stainless steel elbow on the drain tubing on the left side of the Cold Trap.



When draining the CentriVap Cold Trap always attach the other end of the grounding clip to the solvent catch pot to eliminate the risk of electrostatic spark ignition.



Solvent Safety Precautions

The CentriVap is not classified as “explosion proof.” It has been designed with safety as a primary consideration and should be used in a prudent manner using “good laboratory practices.” It has been designed for use with compounds as described in the United States National Electrical Code Class I, Group D. The heater may be programmed to run as hot as 100°C, however, the heater element may normally run at 110°C. A thermal fuse limits the heater to a maximum temperature of 141°C. It is important that the solvents used are compatible with these temperatures. Do not evaporate solvents that have an autoignition temperature below 180°C. Do not evaporate solvents that are classified as Group A, B, or C by the National Electrical Code. Evaporate only non-flammable or Group D solvents with autoignition temperatures 180°C or above. Use of other compounds could cause an explosion.

Solvents used in the CentriVap may be flammable or hazardous. Use extreme caution and keep sources of ignition away from the solvents. When using flammable or hazardous solvents, both the CentriVap and the vacuum pump should be operated inside a fume hood.

If a sample is spilled in the chamber it must immediately be cleaned up. Hazardous materials such as strong acids or bases, radioactive substances and volatile organics, must be handled carefully and promptly cleaned up if spilled.

Do not store flammable or hazardous solvents within 12 inches (300 mm) of the CentriVap.

Several components of the CentriVap which are located inside the chamber are made of stainless steel which can be attacked by acids. Use of acids such as trifluoroacetic acid can result in degradation of the product and the vacuum pump. Use care when using aggressive liquids which can damage the CentriVap and thoroughly clean the CentriVap after each use. Contact Labconco before evaporating acids.

WARNING: The disposal of substances used in connection with this equipment may be governed by various Federal, State or local regulations. All users of this equipment are urged to become familiar with any regulations that apply in the user's area concerning the dumping of waste materials in or upon water, land or air and to comply with such regulations.

Your Next Step

The installation and setup of your CentriVap is now complete. To learn how to load and operate your CentriVap, proceed to *Chapter 4: Using Your CentriVap*. To make a modification to the configuration of your CentriVap, proceed to *Chapter 6: Modifying your CentriVap*. To perform additional diagnostics on your CentriVap, proceed to *Chapter 7: Troubleshooting*. To learn about the maintenance requirements for your CentriVap, proceed to *Chapter 5: Maintaining Your CentriVap*.

CHAPTER 4

USING YOUR

CENTRIVAP

After your CentriVap has been installed as detailed in *Chapter 3: Getting Started*, you are ready to begin using your CentriVap. Read this chapter to learn how to:

- set operating parameters.
- operate the controls.
- properly select and position glassware inside your CentriVap.
- understand the display.
- interrupt a cycle after it has begun.



Do not use the CentriVap in a manner not specified by the manufacturer (refer to *Appendix C: CentriVap Specifications*). The electrical protection properties of the CentriVap may be impaired if the CentriVap is used inappropriately.



Do not store or stack supplies or equipment on top of the CentriVap.

Planning

Thoroughly understand procedures and the equipment operation prior to beginning work. The unique performance of the CentriVap is dependent upon the proper balance of heat, vacuum and centrifugal force. If the proper balance is not established, it is possible to damage or lose a portion of the sample. Therefore, if you are unfamiliar with the CentriVap or are attempting a new protocol, it may be helpful to make a trial run that is void of the sample you are attempting to concentrate.

Glassware Selection

Normally, sample tubes should be filled no more than approximately half full. Select the size of the sample tube so it is compatible with the rotor and the desired sample size. Tubes should not be loose in the rotor. Rotors are available with holes for various size tubes. Refer to *Appendix D: CentriVap Accessories* for available rotor sizes.

Loading Glassware Into the CentriVap

Smooth operation of the CentriVap is dependent upon proper balance of the machine. Therefore, if less than a full load of samples is run, it is important to load samples into the CentriVap in a fairly symmetrical manner distributing the weight of the samples evenly in the sample rotor.

Heat Setting Guidelines

The evaporation rate achieved by the CentriVap is dependent upon a variety of factors. These include the nature of the solvent, the temperature and the pressure in the vacuum system.

As a general guideline, to speed the evaporation process, the CentriVap temperature should be set as high as possible as long as the temperature will not damage the sample or cause the sample to bump.

Time Setting Guidelines

The CentriVap Concentrator has two timers. The “RUN TIME” turns the entire concentrator off after the user set period of time. This stops the rotation, turns off the heater and vacuum pump and bleeds vacuum from the system. The heater may be turned off prior to the concentrator turning off so heat sensitive samples may be protected from exposure to excessive heat after the solvent has evaporated. To turn the heater off prior to stopping the entire system, enter a set time into the memory at the “HEATER TIME”. When the programmed time expires, the heater will turn off but the rotation and vacuum will continue until the run time expires.


The tables in *Appendix C: CentriVap Specifications* indicate approximate times required to evaporate various common solvents. Actual times must be determined by the user. The CentriVap can be set to alarm after a preset period of operation. When the time expires, the CentriVap will give an audible alarm and turn itself off.

Heat Boost Operation

Some CentriVap models are equipped with a secondary “Heat Boost” heater which is positioned on the side wall of the chamber near the top. It provides additional heat to the samples to speed evaporation. The “Heat Boost” heater is controlled by the microprocessor to maintain the set point temperature at the bottom of the chamber to prevent excessive overheating of the samples.

CentriVap Controls

The control panel for the CentriVap is shown below with a description about its function.

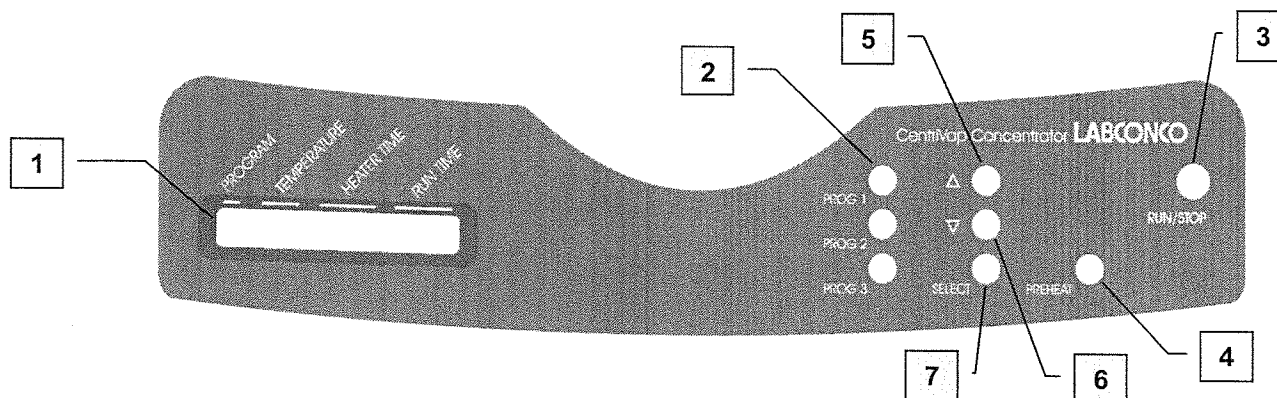

1. Display – The liquid crystal display (LCD) shows set point parameters and actual measured conditions.
2. Program Buttons – Used to initiate the start of a run with the use of just one button.
3. Run/Stop Button – Used to start or stop a run.
4. Preheat Button – Used to turn on the heater to preheat the chamber prior to loading samples.
5. Increase Button – When pressed, the last selected set point will increase.
6. Decrease Button – When pressed, the last selected set point will decrease.
7. Set Point Select Button – To select a parameter to change, press the select button. Arrows on the display will point to the parameter that may be altered.
8. Heat Boot Button (not shown) – If the model is so equipped, pressing the button will activate or deactivate the auxiliary Heat Boost heater.

Operating The CentriVap Controls

Preheat:

To preheat the chamber, press the "PREHEAT" button. The display will show:

SP: XXX ACT: XXX

Press the increase or decrease button until the desired set point (SP) is displayed. The actual chamber temperature, (ACT) is displayed to the right. When power is being supplied to the heaters, a bar under the actual temperature will illuminate. The chamber will continue to preheat until either the "PREHEAT" button is pressed again or the "RUN" button is pressed.

Select existing program:

Operating parameters can be stored in memory so protocols can be repeated. Nine programs can be stored. To select a program, press the set point "SELECT" button until arrows point to the program number indicating that this set point can be run or altered. To change the program number, press the increase or decrease button until the desired program number is displayed. When the program number is changed, all its set points change also to indicate the last entered parameters for that program.

Store frequently run protocols in program 1, 2, or 3. Then, by pressing "PROG 1", "PROG 2" or "PROG 3", the stored program will be initiated without having to press any other button. Pressing just the one button starts the rotor, the heater, the timers and the vacuum pump.

Change heat set point:

To change the heat set point, press the set point “SELECT” button until arrows point to the temperature set point which can be changed from -- (OFF) up to 99° by pressing the increase or decrease buttons. The set point is 100°C if the display shows “HI.” The last entered set point is stored in memory.

Change run time or heater time set point:

To change the time set point, press the set point “SELECT” button until arrows point to the run time set point which can be changed from 1 to 999 minutes by pressing the increase or decrease buttons. If it is desired to have the CentriVap run continuously without alarming at the end of a time period, press the increase button until the display says “ON.” The last entered set point is stored in memory.

If during a run the “STOP” button is pressed, the timers remember the time at which stop occurred. If “RUN” is then pressed, the timers continue to count down from the time at which they were stopped. If you are running program 1, program 2 or program 3, pressing “PROG 1”, “PROG 2” or “PROG 3” resets the timers to the original set point time and the CentriVap starts a new run.

To reset the timers to the original set point time when running programs other than program 1, program 2 or program 3, press the start button and hold it for five seconds. The display will indicate that the timer is reset.

Operating The CentriVap



Never lift the lid if the rotor is moving.

Never attempt to reach into the chamber if the rotor is moving.

Never attempt to defeat the lid latch mechanism.

Do not operate the CentriVap if the lid is scratched or nicked, or shows signs of damage.

Never lean on the CentriVap when it is operating.

1. Press the Cold Trap "ON" switch. The "READY" indicator will illuminate when it reaches operating temperature.
2. Select a program or set the set point parameters.
3. Preheat the chamber if desired.
4. Turn on Heat Boost if the CentriVap is so equipped and additional heat is desired.
5. Place samples in vials. Normally the vials should be no more than half full. Place vials in a rotor.
6. Load the rotor with samples into the chamber.
7. Close the lid.
8. Press "RUN." If the display was showing set point parameters, it will change to show actual parameters. Press "RUN" again. The "S" (STOP) in the display changes to "R" (RUN). The program on the display alternately displays "R" or the number of the program that is running. If you intend to run program 1, 2 or 3, simply press "PROG 1", "PROG 2" or "PROG 3" to quick start the CentriVap. The rotor will start, the vacuum break valve will close and the vacuum pump will start after the rotor reaches operating speed.
9. Set point parameters can be altered at any time during a run by first selecting the parameter using the set point "SELECT" button and then pressing the "INCREASE" or "DECREASE" switch.
10. If the time set point is used, at the end of the set time an alarm sounds. All functions cease.
11. Press "STOP" to terminate operation if the CentriVap has not already stopped itself.
12. When the evaporation is complete, allow the rotor to stop moving, lift the lid and remove the samples.

Operational Notes

As solvent is evaporated in the Concentrator and then condensed in the Cold Trap, it is normal for the Cold Trap temperature to rise as its load increases.

Depending on which solvent is used, the volume of the sample and the system operating parameters, the Cold Trap may warm up sufficiently to cause the “READY” indicator to turn off. As the sample reaches completion, the load on the Cold Trap will decrease and its temperature will decrease. The “READY” indicator will once again illuminate.

The LCD display conveys various pieces of information. When the CentriVap is turned on, the CentriVap returns to the same mode (“RUN” or “STOP”) that it was in when the power was turned off. If the CentriVap was in the “RUN” mode when the power was turned off, when the power is turned on, the CentriVap attempts to return to the programmed set points and continue the run.

Interrupting a Cycle After it Has Begun

At any time during a run, the cycle may be stopped by pressing the “STOP” button. This shuts off all operating functions. After the rotor stops, the lid may be opened. If it is necessary to re-start the CentriVap, close the lid and press “RUN.” The CentriVap resumes operation at the same set point parameters and the timer continues to count down from the time at which the CentriVap was stopped.

CHAPTER 5

MAINTAINING YOUR

CENTRIVAP

Under normal operation, the CentriVap requires little maintenance. The following maintenance schedule is recommended:

As needed:

1. Clean up all spills; remove liquids from the chamber. Clean or decontaminate all surfaces using agents suitable for the substance spilled.
2. Clean lid and gasket using soft cloth, sponge or chamois and a mild, non-abrasive soap or detergent.
3. Check oil level of the vacuum pump, if applicable. It should be between MIN and MAX. If the oil level is less than an inch (25.4 mm) above MIN, add oil to proper level.
4. If oil shows cloudiness, particles or discoloration, drain the pump and replace with fresh oil.
5. Utilization of acids requires immediate cleaning and neutralization after a run or physical damage to the collection chamber will result.
6. Check the Cold Trap for condensed or frozen solvents and dispose of appropriately. Completely empty the trap before the next run. If solvents are frozen in the glass trap, run it under cold water immediately after operating.



IF THE ICE HAS MELTED, THE GLASS TRAP INSERT MUST BE EMPTIED BEFORE THE COLD TRAP IS STARTED AGAIN.

7. If the Glass Trap is used, check to see that the ethanol in the stainless steel trap is free of ice or water. Drain the ethanol and replace it with fresh ethanol.
8. If the media in the optional clear canister has changed color, discard and replace the insert with a new insert. For the radiochemical trap insert, no indicator exists; therefore, it should be discarded after each use. In radioactive applications, the system should be monitored with a Geiger counter.

Monthly:

1. The rubber components on the CentriVap may eventually deteriorate and require replacement. The effective life of rubber parts depends upon both their usage and the surrounding environment. Check all rubber hoses and gaskets and replace any that show signs of hardening, permanent set or deterioration.
2. Using a soft cloth, sponge or chamois and a mild, non-abrasive soap or detergent, clean the glass lid.
3. Using a soft cloth, sponge, or chamois and a mild, non-abrasive soap or detergent, clean the exterior surfaces of the unit. Liquid spray cleaners and polishes may be used on the exterior surfaces. Do not use solvents to remove stains from the exterior surfaces as they may damage the finish.

Annually:

1. Every 12 months, or more often, if the Cold Trap is operated in a dusty environment, the refrigeration system condenser of the Cold Trap should be cleaned. Using a vacuum cleaner with brush attachment, clean the condenser to ensure proper airflow for peak performance.

CHAPTER 6

MODIFYING YOUR

CENTRIVAP

The configuration of your CentriVap can be changed to accommodate your needs. If the solvents used in the CentriVap degrade the acrylic lid it may be replaced with an optional glass lid to gain added chemical resistance. You may wish to add a secondary trap to trap vapors exhausted from the vacuum pump. To observe the samples while they are processing, an optional strobe light may be installed. Read this chapter to learn how to:


- install a glass lid
- install a chemical trap.
- install a CentriZap™ strobe.
- install a glass trap in the Cold Trap chamber.

Installing a Glass Lid

Turn off the CentriVap. Unplug the power cord from the wall receptacle. Pull outward on the hinge pin knob. Lift and remove the old lid. To install the new lid, reverse the process.

Installing a Secondary Chemical Trap

An accessory secondary chemical trap is available to minimize the exhausting of solvents into the atmosphere. It may be attached to either side of the Cold Trap. After selecting the side, remove the two small plastic hole plugs. Attach the bracket to the side of the Cold Trap housing using the screws provided. Attach the hose from the Cold Trap Lid Assembly to the "out" connector of the canister housing. Connect another hose from the remaining fitting on the Secondary Trap to the inlet port on the vacuum pump. Clamp hoses securely. Unscrew the clear bowl of the canister housing from the head. Remove both the upper and lower caps from the filter cartridge and insert the small end of the cartridge into the hole in the center of the head. Reinstall the clear bowl.

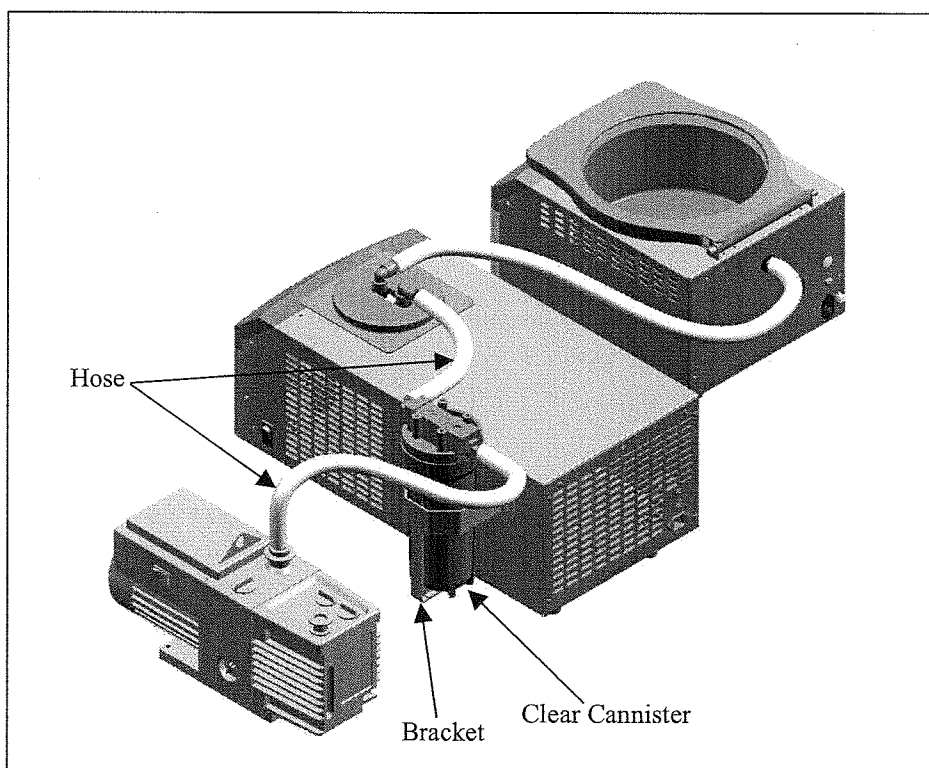

Be sure to use the proper cartridge for your application. The moisture cartridge is used to trap water vapor. The acid cartridge is used to trap acid vapors. The solvent cartridge is used to trap solvent vapors and the radiochemical cartridge is used to trap radioactive waste.

When the media in the insert has changed color, discard the insert and replace it with a new insert. For the radiochemical trap insert, no color indicator exists, therefore it should be discarded after each use. Use a Geiger counter to monitor the pump exhaust.




THIS RADIOCHEMICAL
CARTRIDGE DOES NOT MEET
NRC FILTER DESIGN
RECOMMENDATIONS.

AFTER OPERATING, PROPERLY
DISPOSE OF ALL HAZARDOUS
MATERIALS IN COMPLIANCE
WITH ALL APPLICABLE CODES.
LABCONCO IS NOT RESPONSIBLE
FOR IMPROPER DISPOSAL OF ANY
MATERIALS.

Installing a CentriZap™ Strobe Light

An accessory strobe light is available to enable you to see the samples as they are rotating in the rotor. Attach the holder to the right hand side of the CentriVap Concentrator using the screws provided. Plug the connector on the strobe light harness into the receptacle on the back of the CentriVap marked "STROBE OUTLET." Peel the protective backing off the enclosed Velcro® and attach it to the back of the Concentrator. Secure the power supply box on the harness to the Velcro. Place the light in the holder.

To use the strobe light while the CentriVap is operating, remove the light from its holder, press the trigger and shine the light on the samples in the rotor.

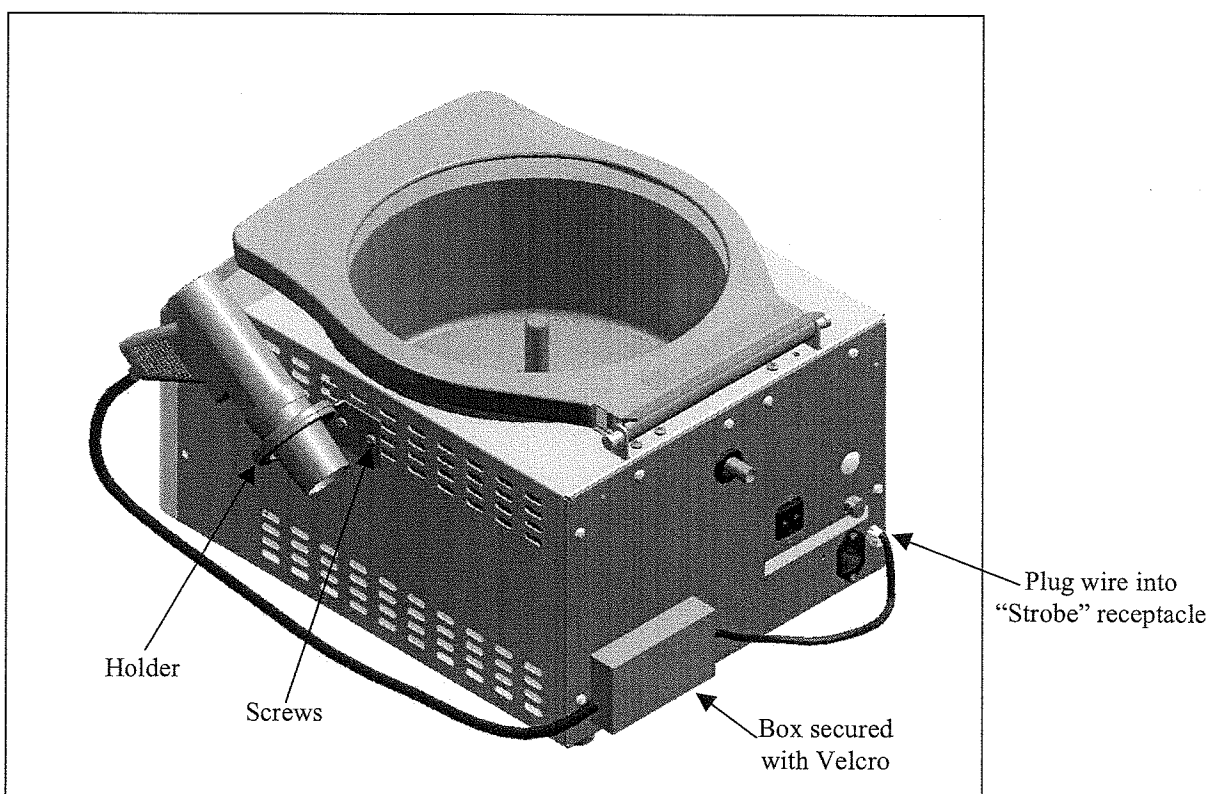


Installing a Glass Trap in the Cold Trap

An accessory Glass Trap is available for use in the Cold Trap for use when corrosive chemicals are used that could attack the stainless steel chamber of the Cold Trap. Disconnect the clamps and remove the Cold Trap Lid Assembly. Attach the hose from the Concentrator to the barb fitting on the center tube of the Glass Trap and clamp securely. Attach the hose from the vacuum pump or Secondary Trap to the other barb fitting on the Glass Trap and clamp securely. Place the Glass Trap inside the stainless steel trap. Be certain that the drain valve is closed. Add ethyl alcohol to the stainless steel trap until the Glass Trap is at least two-thirds immersed. Fit the Glass Trap insulation tightly around the top opening of the stainless steel trap to hold the Glass Trap securely in place.



AFTER A RUN, IF THE ICE IN THE GLASS TRAP HAS MELTED, THE TRAP MUST BE EMPTIED BEFORE THE COLD TRAP IS STARTED AGAIN.

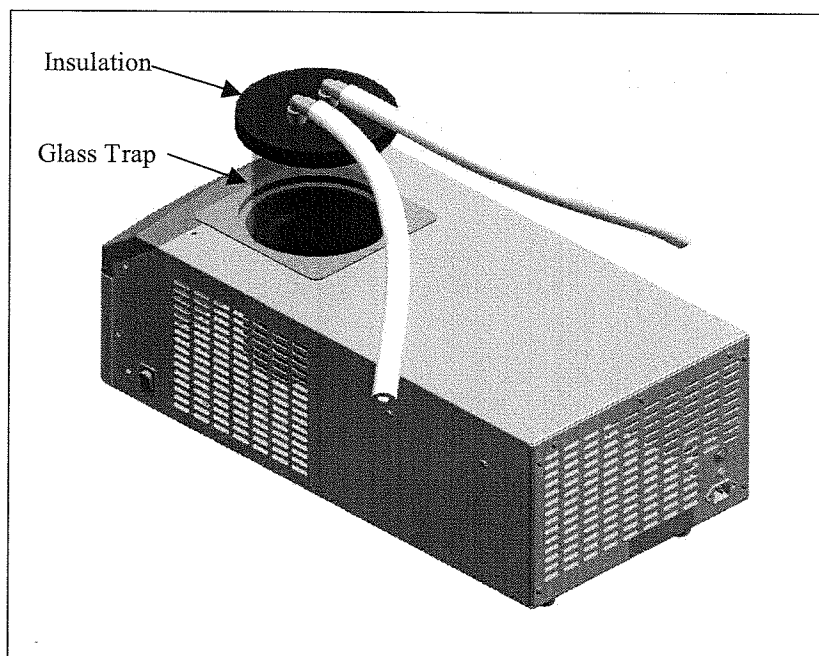

CHAPTER 7

TROUBLESHOOTING

Refer to the following if your CentriVap fails to operate properly. If the suggested corrective actions do not solve your problem, contact Labconco for additional assistance. The following failure codes may appear on the display when problems are sensed by the internal self check routine.

DISPLAY ERROR CODE	CAUSE	CORRECTIVE ACTION
HEAT SENSOR	Sensor failure	Replace sensor assembly.
	Connection failure	Repair connection.
CLOSE LID	Lid open	Close lid.
LATCH FAIL	Solenoid failure	Check component.
	Switch or sensor failure	Check connections.
MEM FAIL P1	Memory failure	Push program button #1
	New memory IC chip	Push program button #1.
	Bad memory IC chip	Call Labconco – Replace IC chip or control PCB.
MOTOR ERROR	Defective motor	Replace motor.
	Hall effect sensor failure	Replace sensor.
	Wire failure	Replace wire.

Other corrective actions for potential problems are as follows:

PROBLEM	CAUSE	CORRECTIVE ACTION
Unit will not operate	Unit not connected to electrical power	Connect unit to proper electrical receptacle.
	Circuit breaker blown	Correct electrical problem and reset circuit breaker by pressing button.
	Lid open	Close lid.
Excessive vibration	Sample tubes not located symmetrically in rotor	Reposition sample tubes.
Sample odor in lab	Vent hose exhausting into lab area	Redirect hose to fume hood.
Evaporation rate is reduced	Heater inoperable	Contact Labconco.
	Vacuum pump failure	Check pump.
	Obstruction in hose	Remove obstruction or replace hose.
	Lack of adequate vacuum	See below.
No vacuum poor vacuum	Pump not on	Turn on pump.
	Control valve open	Check control valve.
	Leaks in lines or connectors or gasket	Locate and repair.
	Foreign material on lid gasket	Clean gasket and lid.
	Pump is not functioning properly	Check pump by locating vacuum gauge closer to pump and close off rest of system. Check pump oil for cloudiness or particles and change. If pump is faulty, seek authorized service or replace pump.
	Cold Trap or Concentrator gasket is not sealing properly	Check gasket for cleanliness. Adjust gasket as needed.
	Cold Trap lid not seated	Hold lid down until vacuum is initiated.

PROBLEM	CAUSE	CORRECTIVE ACTION
No vacuum poor vacuum (cont.)	Ice formed on Cold Trap lid sealing surface	Defrost and wipe dry.
	Secondary Trap Cannister not fitted properly	Tighten all connections to and from the Secondary Trap Cannister.
	Secondary Trap Insert is spent	Replace with new insert.
	New Secondary Trap has moisture in it	Run vacuum pump for 24 hours to remove moisture.
Recovery of condensate in Cold Trap is less than normally expected	Cold Trap is not ON	Check to make sure switch is ON and condensing unit fan is moving air out of the rear of the cabinet.
	Cold Trap does not cool down	Turn vacuum pump OFF and allow Cold Trap to cool for at least 30 min. to reach temperature. -55°C temperature can be checked with a solvent thermometer or digital thermometer.
Frequent oil change needed in pump	Secondary Trap insert is spent	Change insert often.
	Cold Trap is not emptied after each run and dried	Empty the traps (glass or stainless steel) after each run and replace.
	Vacuum too strong for chemical	Use a Secondary Trap insert and diaphragm pump.
Unit starts and shuts off	Latch optical sensor improperly calibrated	Unplug power cord. Wait 10 seconds. Plug in power cord.

APPENDIX A


CENTRIVAP

COMPONENTS

The following pages list components that are available for your CentriVap. The parts shown are the most common replacement parts. If other parts are required, contact Product Service.


CentriVap Concentrator Components

Item	Quantity	Part No.	Description
1	1	7459000	Motor w/Capacitor
2	1	7481700	Valve, Vacuum Break (115V)
2A	1	7481701	Valve, Vacuum Break (230V)
3	1	7453500	Heater (115V)
3A	1	7453501	Heater (230V)
4	1	1647106	O-Ring, Outer
5	1	1647105	O-Ring, Inner
6	1	7975902	Fuse, High Temp Limiter
7	1	7456000	Harness, Temp & Speed Sensor
8	1	7479400	PCB
9	1	1289200	Relay Vacuum Pump (115V)
9A	1	1289100	Relay Vacuum Pump (230V)
10	1	7826000	Switch, Latch
11	1	7478700	Solenoid, Latch
12	1	7403701	Display
13	1	7455300	Label/Switch Pad
13A	1	7455400	Label/Switch Pad with Heat Boost
14	1	7452600	Gasket, Lid
15	1	7452500	Lid, Acrylic
16	42.2 inch	7451700	Extrusion
17	2	7452200	Hinge, Bracket Assembly
18	1	1289300	Circuit Breaker (115V)
18A	2	1289308	Circuit Breaker (230V)
19	1	1289200	Relay – Heat Boost (115V and 230V)
Not Shown	1	1334500	Power Cord (115V)
Not Shown	1	1334100	Power Cord (230V)

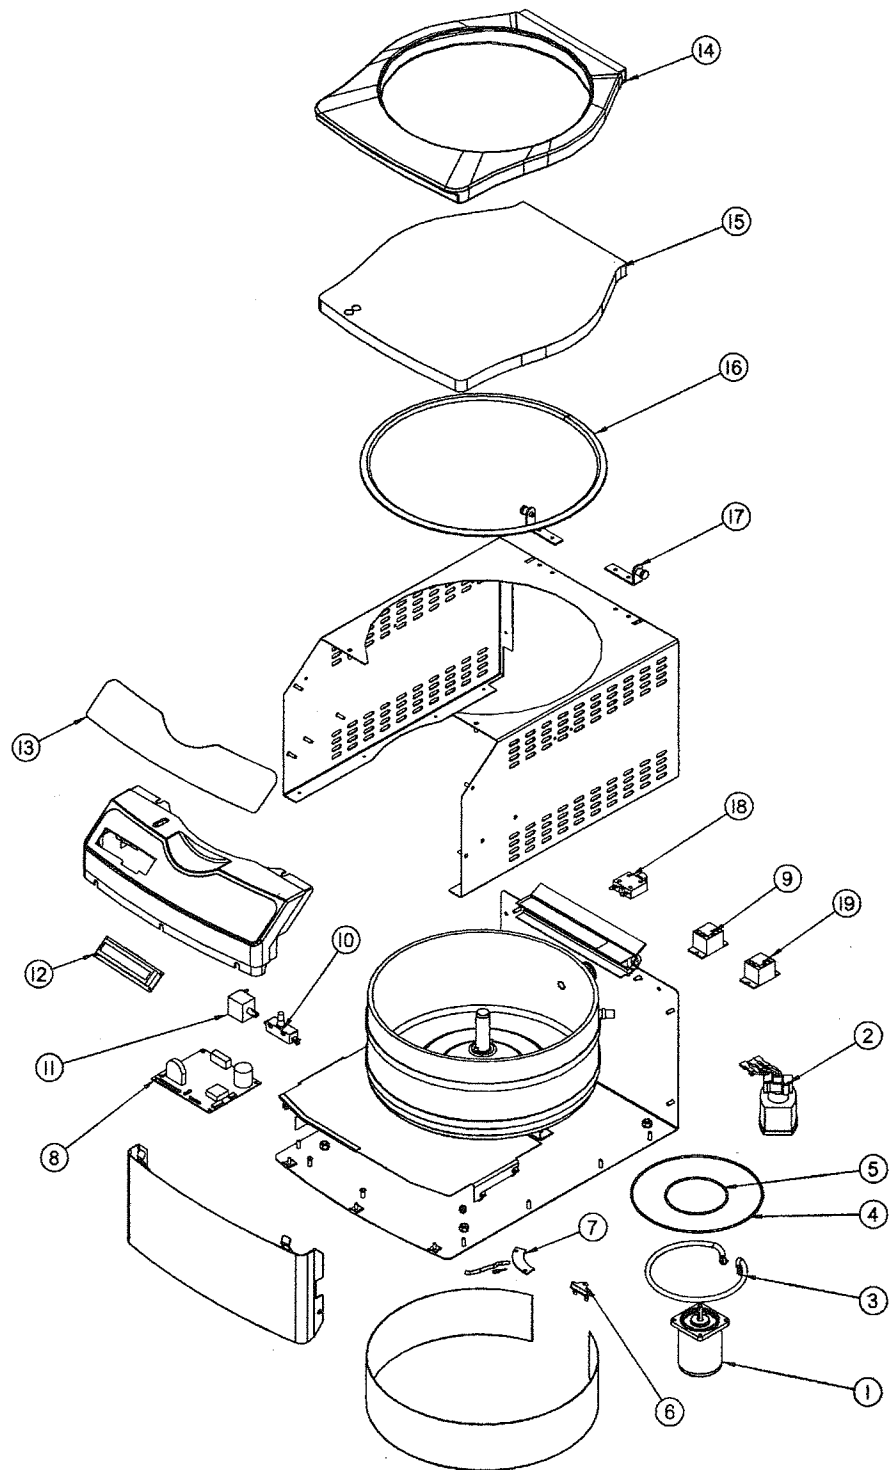


CentriVap Cold Trap Components (-55°C) (Models 78110-00 & 78110-01)

Item	Quantity	Part No.	Description
1	1	7503000	Compressor (115V)
1A	1	7503200	Compressor (230V)
2	1	7936200	Drier
3	1	7463300	Line Assembly
4	1	1302300	Switch
5	1	7463900	Label
6	1	7464405	PCB (LED)
7	1	7464600	Wire Assembly – Ground
8	1	1360500	Valve
9	1	7873500	Cover Assembly
10	2	1548603	Stem Adapter
11	2	1544501	Elbow
12	2	1548101	Stem
13	1	7981400	Insulation – Lid Assembly
13A	1	7873200	Insulation – Glass Trap
14	1	7871500	Glass Trap
15	1	7871000	Gasket
16	1	1327208	Circuit Breaker (115V)
16A	2	1327204	Circuit Breaker (230V)
17	1	1333800	Power Cord Inlet
18		7622202	Refrigerant
19	1	1334500	Power Cord (115V)
19A	1	1334100	Power Cord (230V)
20	1	7464400	PCB (115V)
20A	1	7464402	PCB (230V)

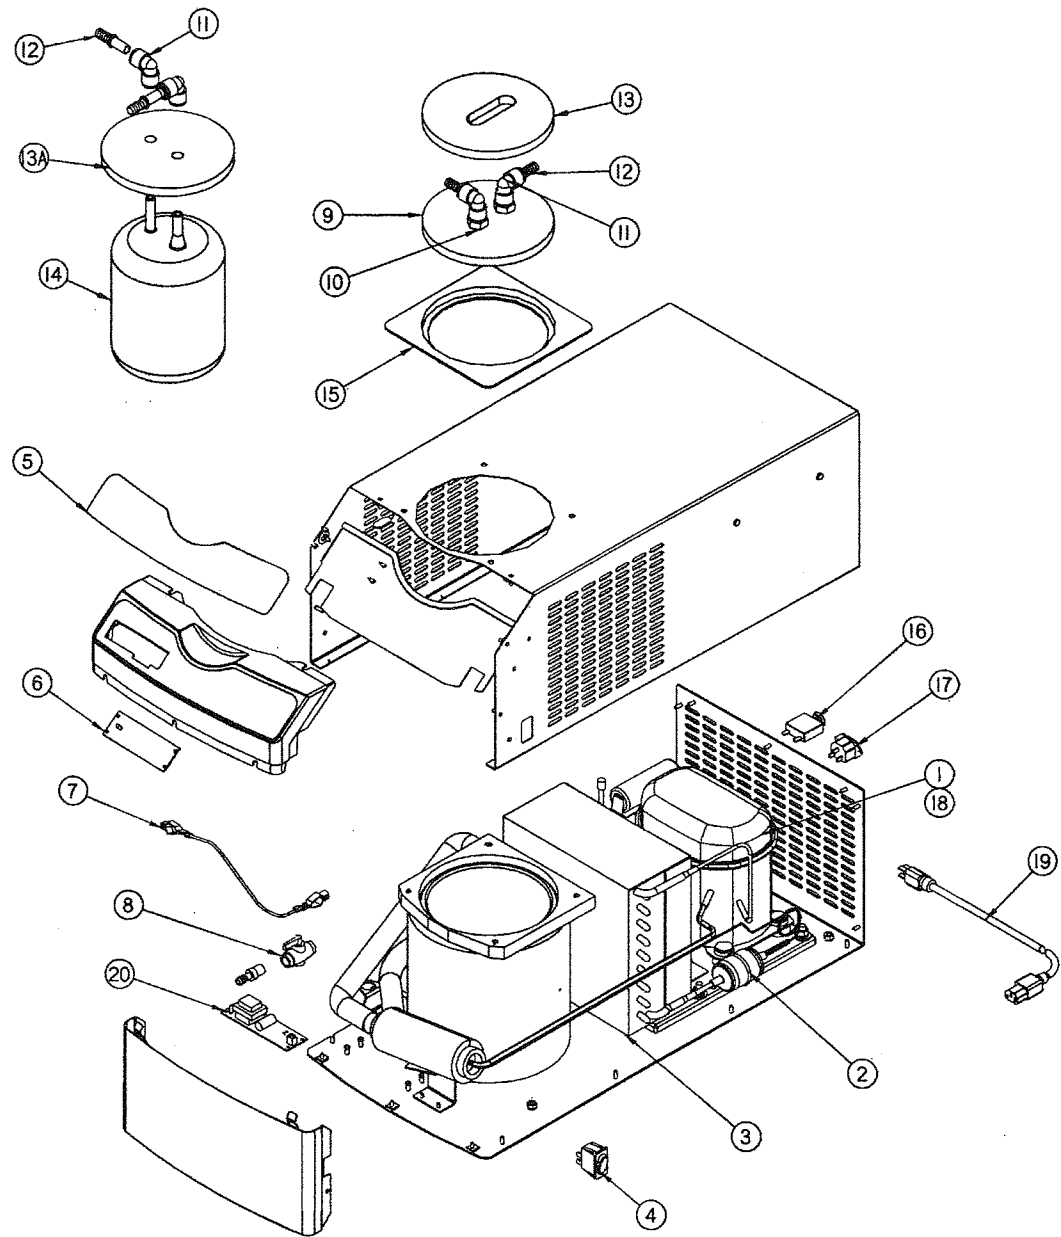

CentriVap Cold Trap Components (-100°C) (Models 74600-00 & 74600-01)

Item	Quantity	Part No.	Description
1	1	7871000	Gasket
2	1	7473000	Label
3	1	7464400	PCB (115V)
3A	1	7464402	PCB (230V)
4	1	1302300	Switch – Power
5	2	7936200	Dryer
6	1	7474200	Timer (115V)
6A	1	7474400	Timer (230V)
7	1	7474500	Switch – Pressure
8	1	1360500	Valve
9	1	7464600	Wire Assembly – Ground
10	1	7873500	Cover Assembly
11	2	1548603	Stem Adapter
12	2	1544501	Elbow
13	2	1584101	Stem
14	1	7981400	Insulation – Lid Assembly
15	1	1334500	Power Cord (115V)
15A	1	1334100	Power Cord (230V)
16	1	1327207	Circuit Breaker (115V)
16A	2	1327208	Circuit Breaker (230V)
17	1	7871500	Glass Trap
18	1	7873200	Insulation – Glass Trap
19	1	1333800	Power Cord Inlet

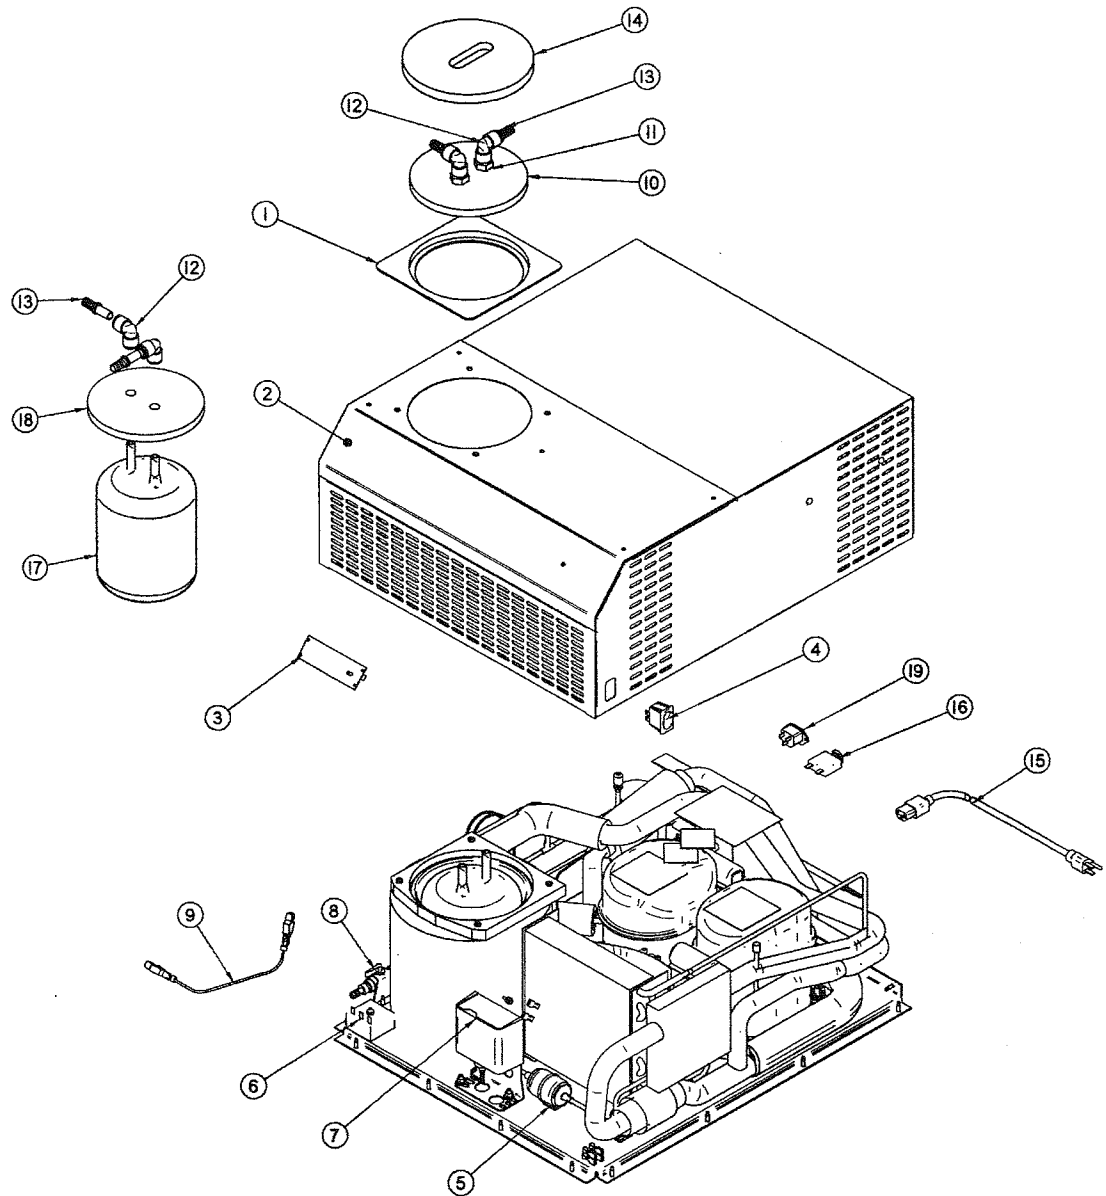


APPENDIX B


CENTRI VAP

DIMENSIONS


CentriVap Concentrator

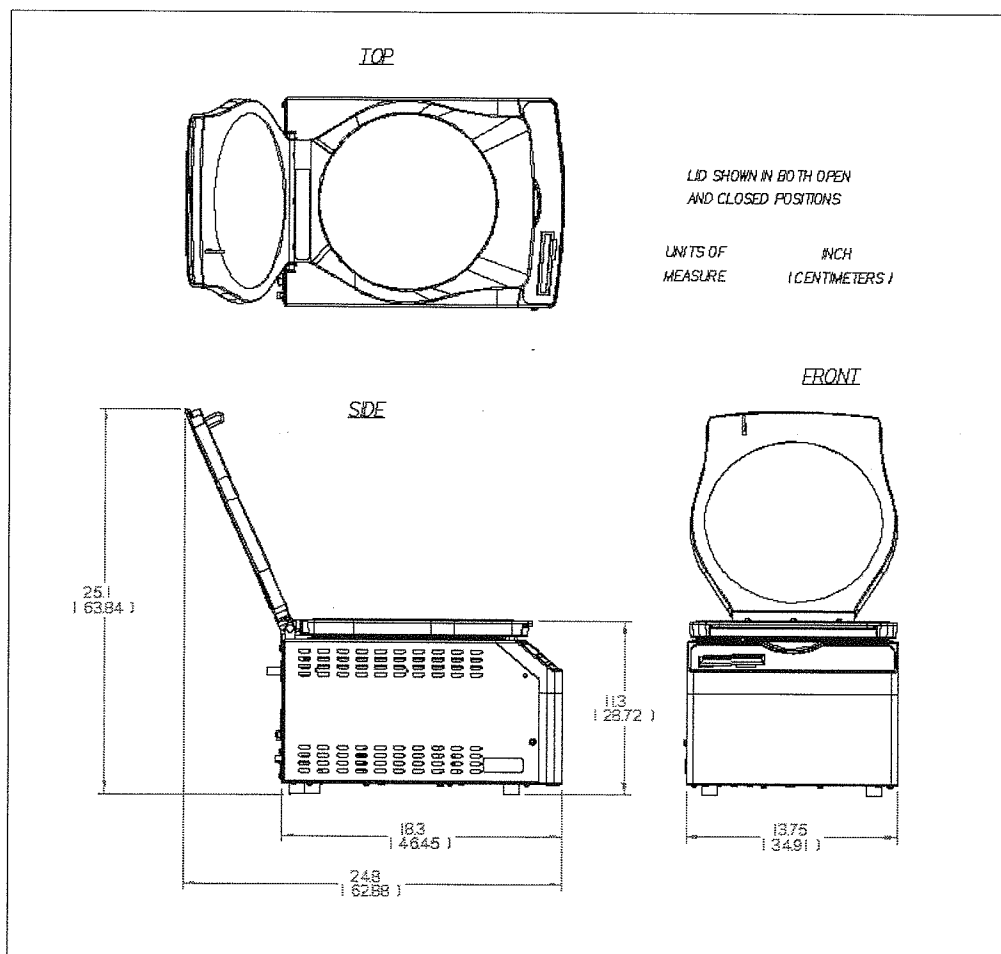

CentriVap Cold Trap (-55°C) (Models 78110-00 & 78110-01)

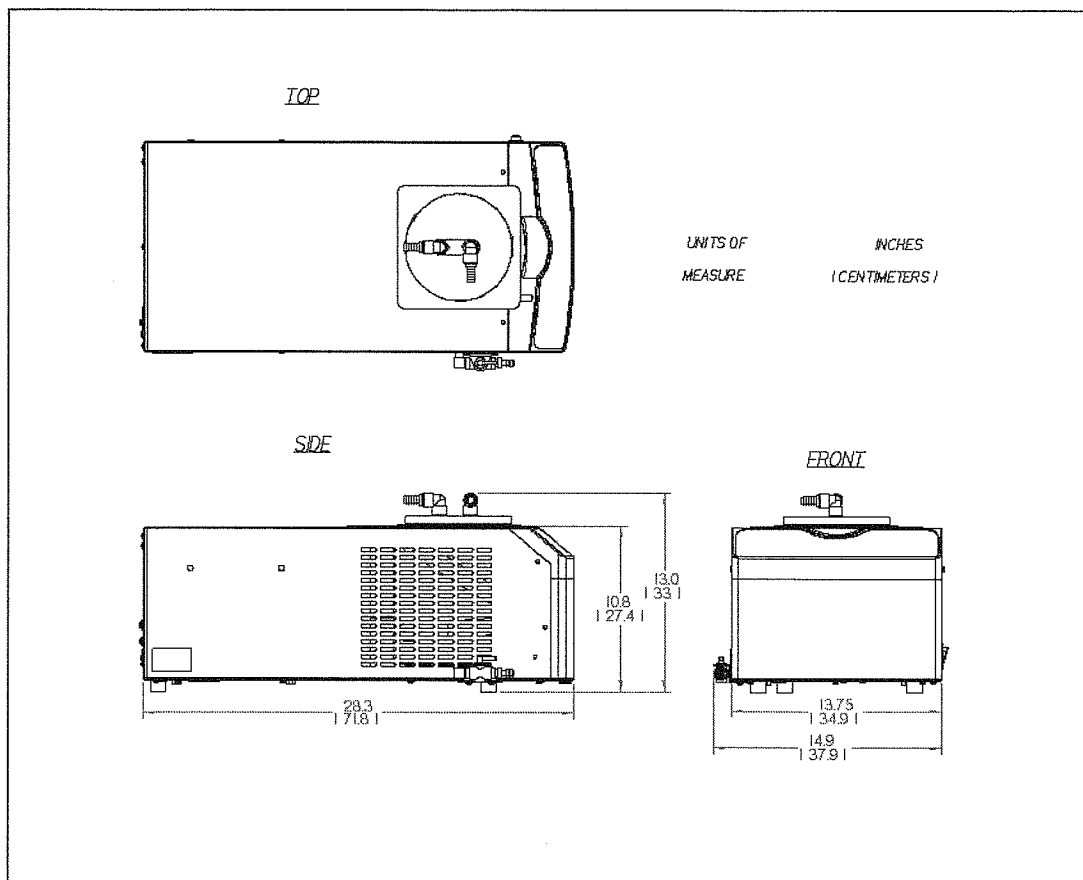

CentriVap Cold Trap (-100°C) (Model 74600-00 & 74600-01)

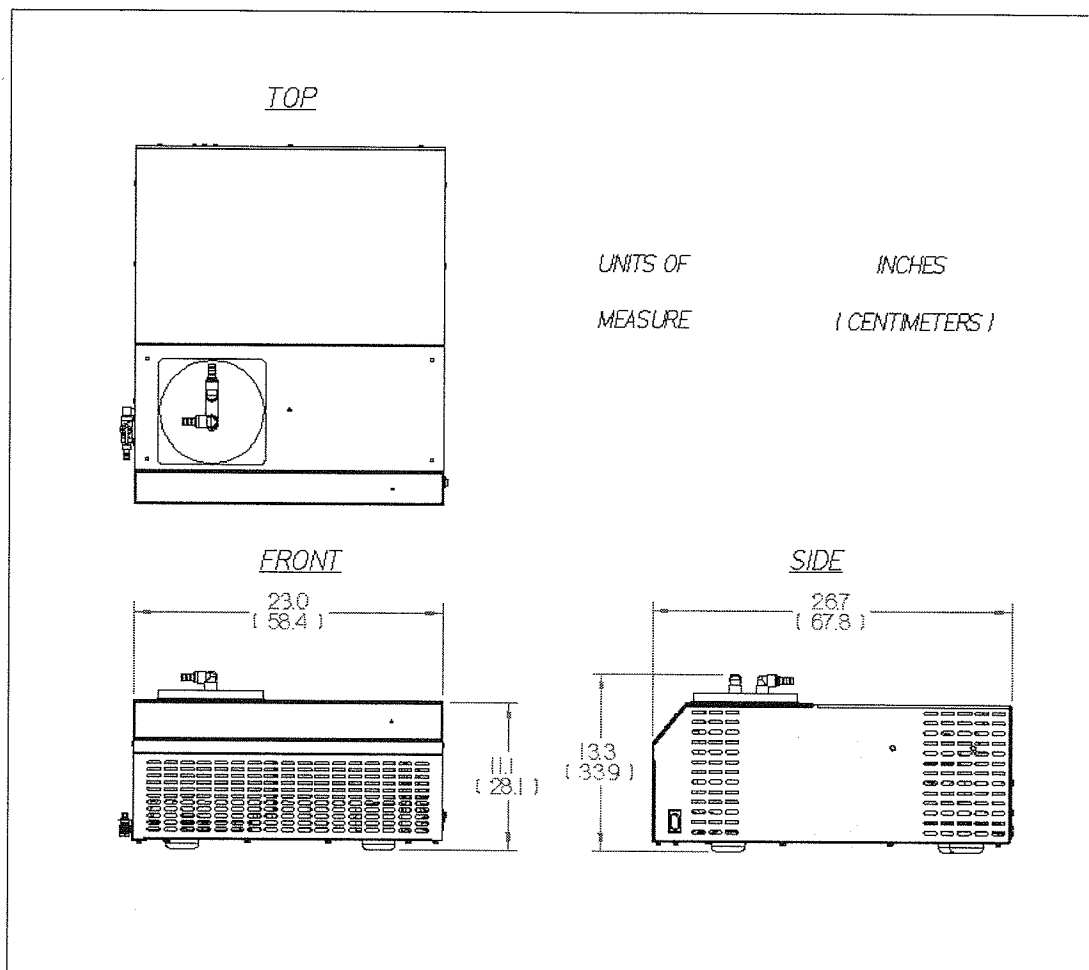

APPENDIX C

CENTRI VAP

SPECIFICATIONS

This Appendix contains technical information about the CentriVap including specifications, environmental operating conditions, wiring diagrams and evaporation rates.


Electrical Specifications


- Nominal amperage for 115V CentriVap Concentrator (model 78100-00) (excluding vacuum pump): 3.1A
- Nominal amperage for 230V CentriVap Concentrator (model 78100-01) (excluding vacuum pump): 1.6A
- Nominal amperage for 115V CentriVap Concentrator (model 78100-02) (excluding vacuum pump): 5.1A
- Nominal amperage for 230V CentriVap Concentrator (model 78100-03) (excluding vacuum pump): 2.6A
- Nominal amperage for 115V Cold Trap (model 78110-00): 5.4A
- Nominal amperage for 230V Cold Trap (model 78110-01): 2.4A
- Nominal amperage for 115V Cold Trap (model 74600-00): 12A
- Nominal amperage for 230V Cold Trap (model 74600-01): 6A
- Frequency: All Concentrators – 50/60 Hz, Cold Traps – 115V/60 Hz or 230V/50 Hz
- Phase: Single

Environmental Conditions


- Indoor use only.
- Maximum altitude: 6562 feet (2000 meters).
- Ambient temperature range: 41° to 104°F (5° to 40°C).
- Maximum relative humidity: 80% for temperatures up to 88°F (31°C), decreasing linearly to 50% relative humidity at 104°F (40°C).
- Main supply voltage fluctuations not to exceed $\pm 10\%$ of the nominal voltage.
- Transient overvoltages according to Installation Categories II (Overvoltage Categories per IEC 1010). Temporary voltage spikes on the AC input line that may be as high as 1500V for 115V models and 2500V for 230V models are allowed.
- Used in an environment of Pollution degrees 2 (i.e., where normally only non-conductive atmospheres are present). Occasionally, however, a temporary conductivity caused by condensation must be expected, in accordance with IEC 664.

53

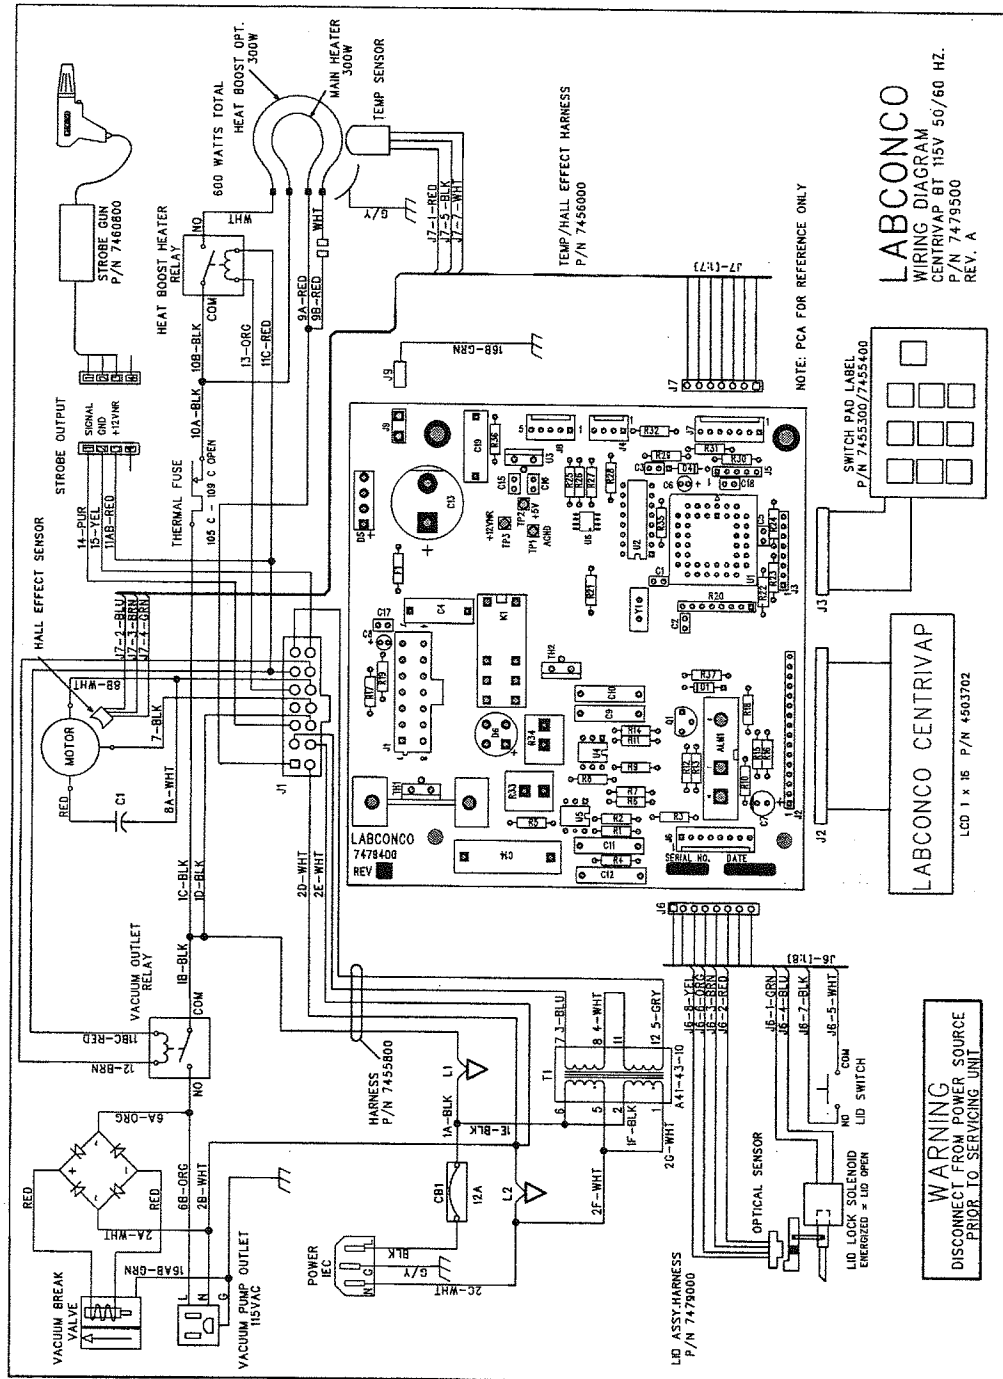


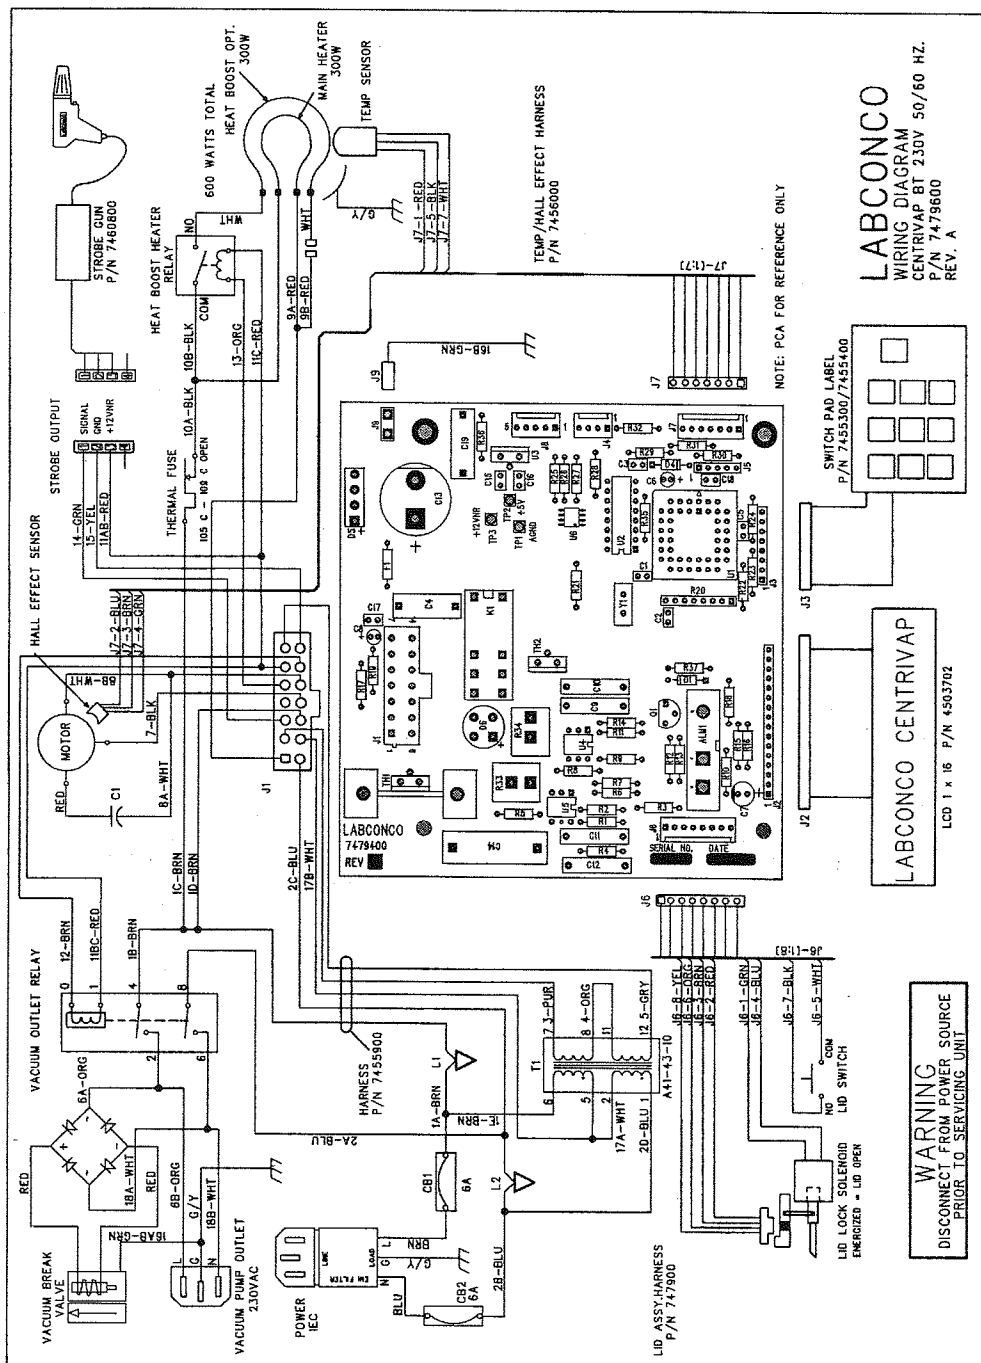

Wiring Diagram Cold Trap (115V & 230V Models) (Models 78110-00 & 78110-01)

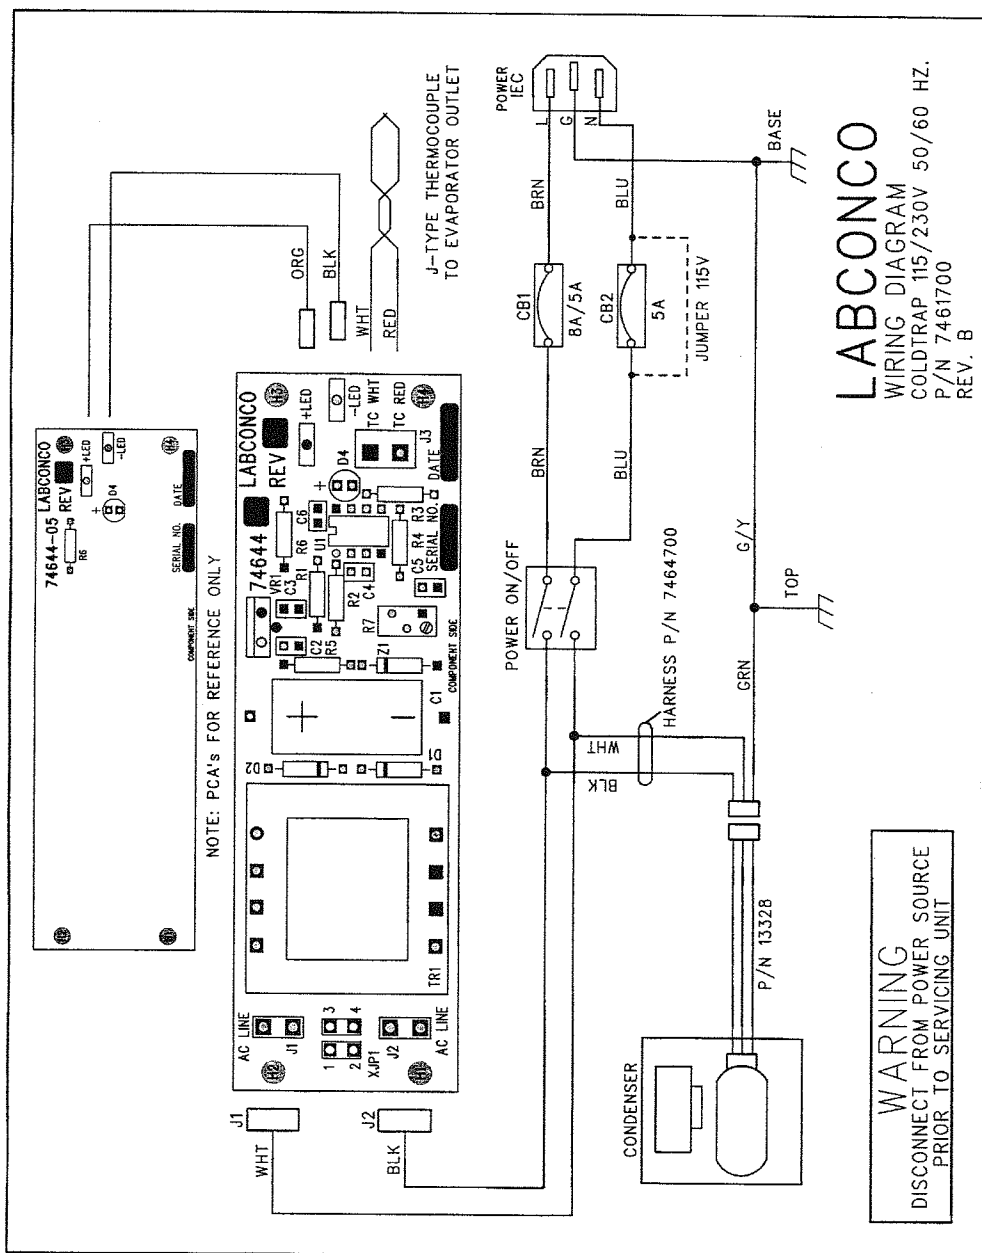

Wiring Diagram Cold Trap (115V & 230V Models) (Models 74600-00 & 74600-01)

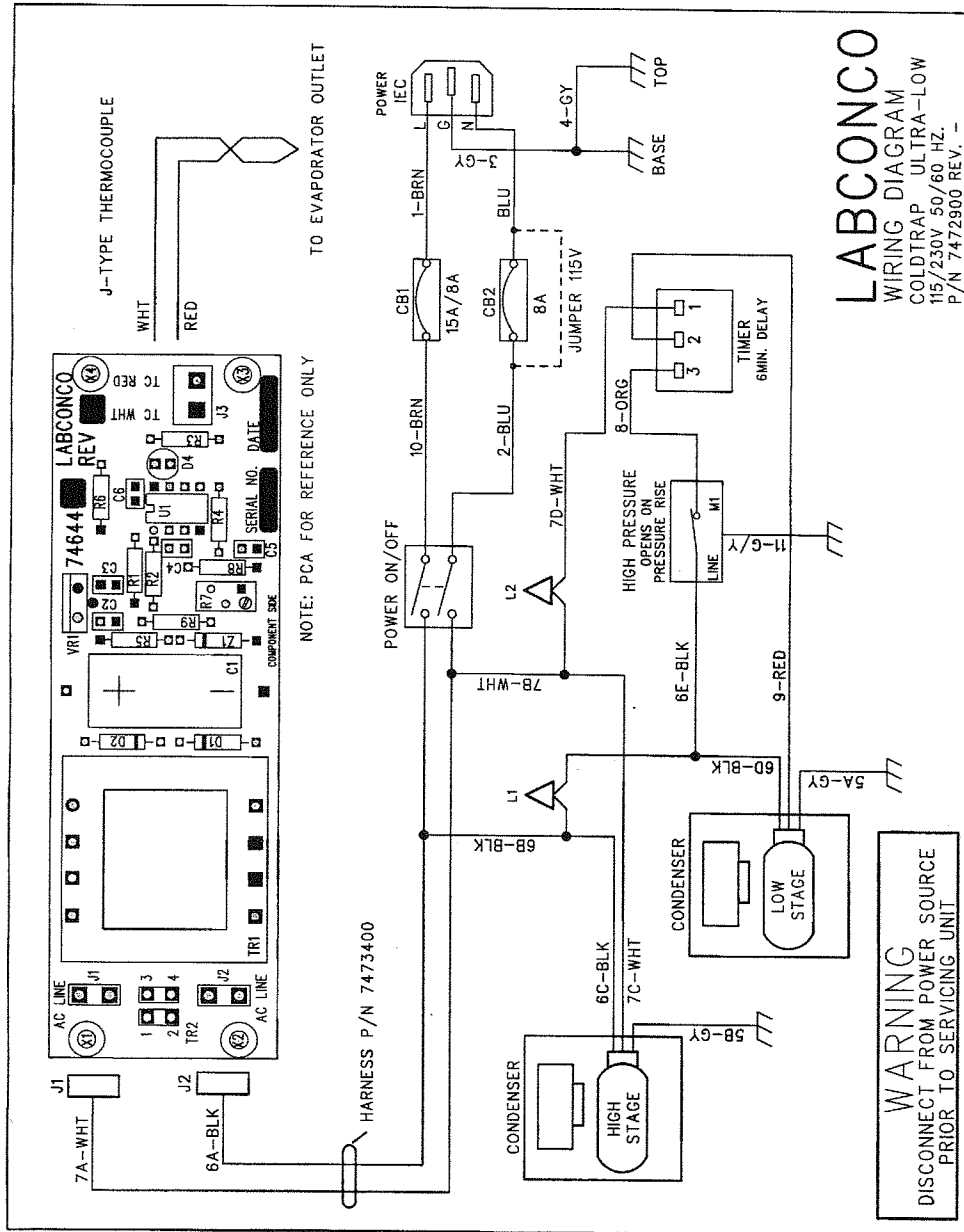

Evaporation Rates

Methylene Chloride bp 40

<i>Tube Size (ml)</i>	<i>Number of Samples</i>	<i>Sample Size (ml)</i>	<i>Heater Temp (C)</i>	<i>Heat Boost</i>	<i>Vacuum Pump</i>	<i>Time to Dry (min)</i>	<i>Cold Trap</i>	<i>Rate Overall (ml/min)</i>
50	12	25	45	off	Diaphragm	80	no	3.75
50	12	25	45	on	Diaphragm	78	no	3.85
15	18	10	45	off	Diaphragm	45	no	4.00
15	18	10	45	on	Diaphragm	45	no	4.00

Toluene bp 111

50	12	25	45	off	Diaphragm	204	no	1.47
50	12	25	45	on	Diaphragm	187	no	1.60
50	12	25	100	off	Diaphragm	96	no	3.13
50	12	25	100	on	Diaphragm	66	no	4.55
15	18	10	45	off	Diaphragm	119	no	1.51
15	18	10	45	on	Diaphragm	99	no	1.82
15	18	10	100	off	Diaphragm	42	no	4.29
15	18	10	100	on	Diaphragm	34	no	5.29

Acetonitrile bp 82

50	12	25	45	off	Diaphragm	184	no	1.63
50	12	25	45	on	Diaphragm	181	no	1.66
50	12	25	100	off	Diaphragm	81	no	3.70
50	12	25	100	on	Diaphragm	77	no	3.90
15	18	10	45	off	Diaphragm	106	no	1.70
15	18	10	100	off	Diaphragm	52	no	3.46
15	18	10	100	on	Diaphragm	45	no	4.00
1.5	132	1	45	off	Diaphragm	55	no	2.40
1.5	90	1	45	off	Diaphragm	47	no	1.92
1.5	132	1	60	off	Diaphragm	37	no	3.57
1.5	132	1	75	off	Diaphragm	33	no	5.74
1.5	132	1	100	off	Diaphragm	21	no	6.29
1.5	132	1	100	on	Diaphragm	17	no	7.76

Methanol bp 65

50	12	25	45	off	Diaphragm	233	no	1.29
15	18	10	45	off	Diaphragm	141	no	1.28
1.5	132	1	35	off	Diaphragm	88	no	1.50
1.5	132	1	45	off	Diaphragm	64	no	2.06
1.5	132	1	60	off	Diaphragm	50	no	2.64
1.5	90	1	75	off	Diaphragm	38	no	2.37
1.5	132	1	75	off	Diaphragm	39	no	3.38
1.5	132	1	100	off	Diaphragm	25	no	5.28
1.5	132	1	100	on	Diaphragm	22	no	6.00

Appendix C: CentriVap Specifications

Water

bp 100

<i>Tube Size (ml)</i>	<i>Number of Samples</i>	<i>Sample Size (ml)</i>	<i>Heater Temp (C)</i>	<i>Heat Boost</i>	<i>Vacuum Pump</i>	<i>Time to Dry (min)</i>	<i>Cold Trap</i>	<i>Rate Overall (ml/min)</i>
50	12	25	45	off	Diaphragm	1397	no	0.21
50	12	25	100	off	Diaphragm	445	no	0.67
50	12	25	100	on	Diaphragm	430	no	0.70
15	18	10	45	off	Diaphragm	841	no	0.19
1.5	132	1	45	off	Diaphragm	427	no	0.30
1.5	132	1	60	off	Diaphragm	303	no	0.44
1.5	132	1	75	off	Diaphragm	196	no	0.67
1.5	132	1	100	off	Diaphragm	117	no	1.13
1.5	132	1	100	on	Diaphragm	108	no	1.22
50	12	25	45	off	rotary vane	1002	yes	0.30
50	12	25	100	off	rotary vane	424	yes	0.70
50	12	25	100	on	rotary vane	373	yes	0.80
15	18	10	45	off	rotary vane	565	yes	0.32
15	18	10	60	off	rotary vane	456	yes	0.39
1.5	132	1	45	off	rotary vane	299	yes	0.44
1.5	132	1	75	off	rotary vane	207	yes	0.64
1.5	132	1	100	off	rotary vane	131	yes	1.01
1.5	132	1	100	on	rotary vane	122	yes	1.08

Vacuum Pumps:

Diaphragm – Rated at 12 mbar ultimate vacuum and 34 L/min displacement

Rotary vane – Rated at 2.0×10^{-3} mbar ultimate vacuum and 195 L/min displacement

Chamber preheated prior to each run to run temp.

APPENDIX D

CENTRIVAP

ACCESSORIES

The following accessories are available for the CentriVap Concentrator and Cold Trap System.

PART #	DESCRIPTION
74629-00	Rotor (DNA) Holds (72) 0.5 ml microcentrifuge tubes and (60) 1.5 ml microcentrifuge tubes or (60) 2.0 ml microcentrifuge tubes
74507-00	Rotor (1.5 ml) Holds (132) 1.5 ml microcentrifuge tubes or (132) 2.0 ml microcentrifuge tubes
74550-00	Rotor (15 ml) Holds (44) 12 x 55 mm tubes or (36) 12 x 75 mm tubes or (36) 12 x 95 mm tubes or (36) 13 x 75 mm tubes or (36) 13 x 100 mm tubes and (24) 16 x 100 mm tubes or (18) 16 x 120 mm conical tubes or (18) 17 x 95 mm tubes or (18) 17 x 100 mm centrifuge tubes or (18) 17 x 120 mm tubes

Appendix D: CentriVap Accessories

PART #	DESCRIPTION
74551-00	Rotor (12 mm) Holds (40) 1.5 ml microcentrifuge tubes or (40) 2.0 ml microcentrifuge tubes and (16) 12 x 55 mm tubes or (100) 12 x 75 mm tubes or (64) 12 x 95 mm tubes or (100) 13 x 75 mm tubes or (64) 13 x 100 mm tubes
74552-00	Rotor (50 ml) Holds (32) 1.5 ml microcentrifuge tubes or (32) 2.0 ml microcentrifuge tubes and (12) 28 x 115 mm conical tubes or (12) 28 x 135 mm conical tubes or (12) 28 x 140 mm conical tubes
74619-00	Rotor (96 well plate) Holds (4) Standard 96 well plates or (2) Deep well 96 well plates
74609-00	Clear Canister - Accommodates inserts listed below
78148-00	Acid Trap Insert
78149-00	Moisture Trap Insert
78150-00	Radiochemical Trap Insert
78152-00	Solvent Trap Insert
74566-01	Glass Lid for Concentrator – Direct replacement for standard equipment acrylic lid. For use with chemicals that could craze acrylic.

PART #	DESCRIPTION
74643-00	Strobe Light – For observing samples while the rotor is spinning.
14721-00	Direct Drive Vacuum Pump – 117 liters/minute pumping capacity with gas ballast. Ultimate pressure 1.3×10^{-4} mBar. 115 VAC, 60 Hz, single phase, 4.6 amp
14677-00	Direct Drive Vacuum Pump – 195 liters/minute capacity with gas ballast. Ultimate pressure 1.3×10^{-4} mBar. 115 VAC, 60 Hz, single phase, 7.8 amp
77394-02	Direct Drive Vacuum Pump – 117 liters/minute. Same as 14721-00 except 220/208-230 VAC, 50/60 Hz, single phase, 2.4 amp operation
77394-03	Direct Drive Vacuum Pump – 195 liters/minute. Same as 14677-00 except 220/208-230 VAC, 50/60 Hz, single phase, 4.0 amp operation
79141-00	Diaphragm Vacuum Pump – Corrosion resistant, 115V, 60 Hz, 3.3 amps, single phase, 42 liters/minute, 23.8 in. Hg vacuum (For use with nonflammable solvents only)
79141-01	Diaphragm Vacuum Pump – Corrosion resistant, 220V, 50 Hz, 1.5 amps, single phase, 35 liters/minute, 23.8 in. Hg vacuum (For use with nonflammable solvents only)
79171-00	Diaphragm Vacuum Pump – Corrosion resistant, 115V, 60 Hz, 10.8 amps, single phase, 88 liters/minute, 29 in. Hg vacuum (For use with nonflammable solvents only)
79171-01	Diaphragm Vacuum Pump – Corrosion resistant, 230V, 50 Hz, 4.5 amps, single phase, 74 liters/minute, 29 in. Hg vacuum (For use with nonflammable solvents only)

7393000

Appendix D: CentriVap Accessories

PART #	DESCRIPTION
79248-00	Diaphragm Vacuum Pump – Corrosion resistant, explosion proof motor, 23.8 in. Hg Vacuum, 115V, 60 Hz, 5.8 amps, single phase, 42 liters/minute
79248-01	Diaphragm Vacuum Pump – Corrosion resistant, explosion proof motor, 23.8 in. Hg Vacuum, 220V, 50 Hz, 3.1 amps, single phase, 36 liters/minute
79249-00	Diaphragm Vacuum Pump – Corrosion resistant, explosion proof motor, 29 in. Hg Vacuum, 115V, 60 Hz, 5.8 amps, single phase, 88 liters/minute
79249-01	Diaphragm Vacuum Pump – Corrosion resistant, explosion proof motor, 29 in. Hg Vacuum, 220V, 50 Hz, 3.1 amps, single phase, 74 liters/minute
14723-00	Vacuum Pump Exhaust Filter – Installs on pumps PN 14721-00, 14677-00, 77394-02 and 77394-03 to eliminate oil mist from the exhaust
75221-00	Two Place Freeze Dry Manifold – Manifold has 1/2" neoprene valves and is used for freeze drying small volume samples
79782-00	Auxiliary Port – Attaches to Cold Trap allowing connection of other laboratory equipment

DECLARATION OF CONFORMITY

Application Council Directive(s): 73/23/EEC, 89/336/EEC

Standard(s) to which conformity is declared: EN60950, EN55014, EN55104

Manufacturer's Name: Labconco Corporation

Manufacturer's Address: 8811 Prospect Avenue
Kansas City, MO 64132 USA

Importer's Name: See Shipping/Customs Documents*

Importer's Address: See Shipping/Customs Documents for your equipment

Type of Equipment: Laboratory Equipment

Model No.: Centrivap DNA System 79700-01
Centrivap Benchtop Concentrator 78100-01, 78100-03
Centrivap Cold Trap 78110-01, 74600-01
Centrivap Mobile Console 78120-01, 78120-03

Serial No.: Various – See Individual Declaration

Year of Manufacture: 2000 and Subsequent

I, the undersigned, hereby declare that the equipment specified above conforms to the above Directive(s) and Standard(s).

See individual Declaration of Conformity which will be signed by the importer for your country.

Place:

(Signature)

Date:

(Full Name)

(Position)

*An individual version of this declaration is included with your shipping/customs documentation.

Labconco P/N 36960-04 Rev. A